

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060721\
 Data File : FG008239.D
 Signal(s) : FID1A.ch
 Acq On : 07 Jun 2021 19:20
 Operator : DD\AJ
 Sample : M2603-25 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 02:01:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.779	609462	5.136 ug/ml
Target Compounds			
7) N-EICOSANE	12.741f	82790	0.605 ug/ml
13) N-TRIACONTANE	17.850	145407	1.139 ug/ml
14) N-DOTRIACONTANE	18.684	185253	1.491 ug/ml
15) N-TETRATRIACONTANE	19.470	115995	0.992 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060721\
Data File : FG008239.D
Signal(s) : FID1A.ch
Acq On : 07 Jun 2021 19:20
Operator : DD\AJ
Sample : M2603-25 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 02:01:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

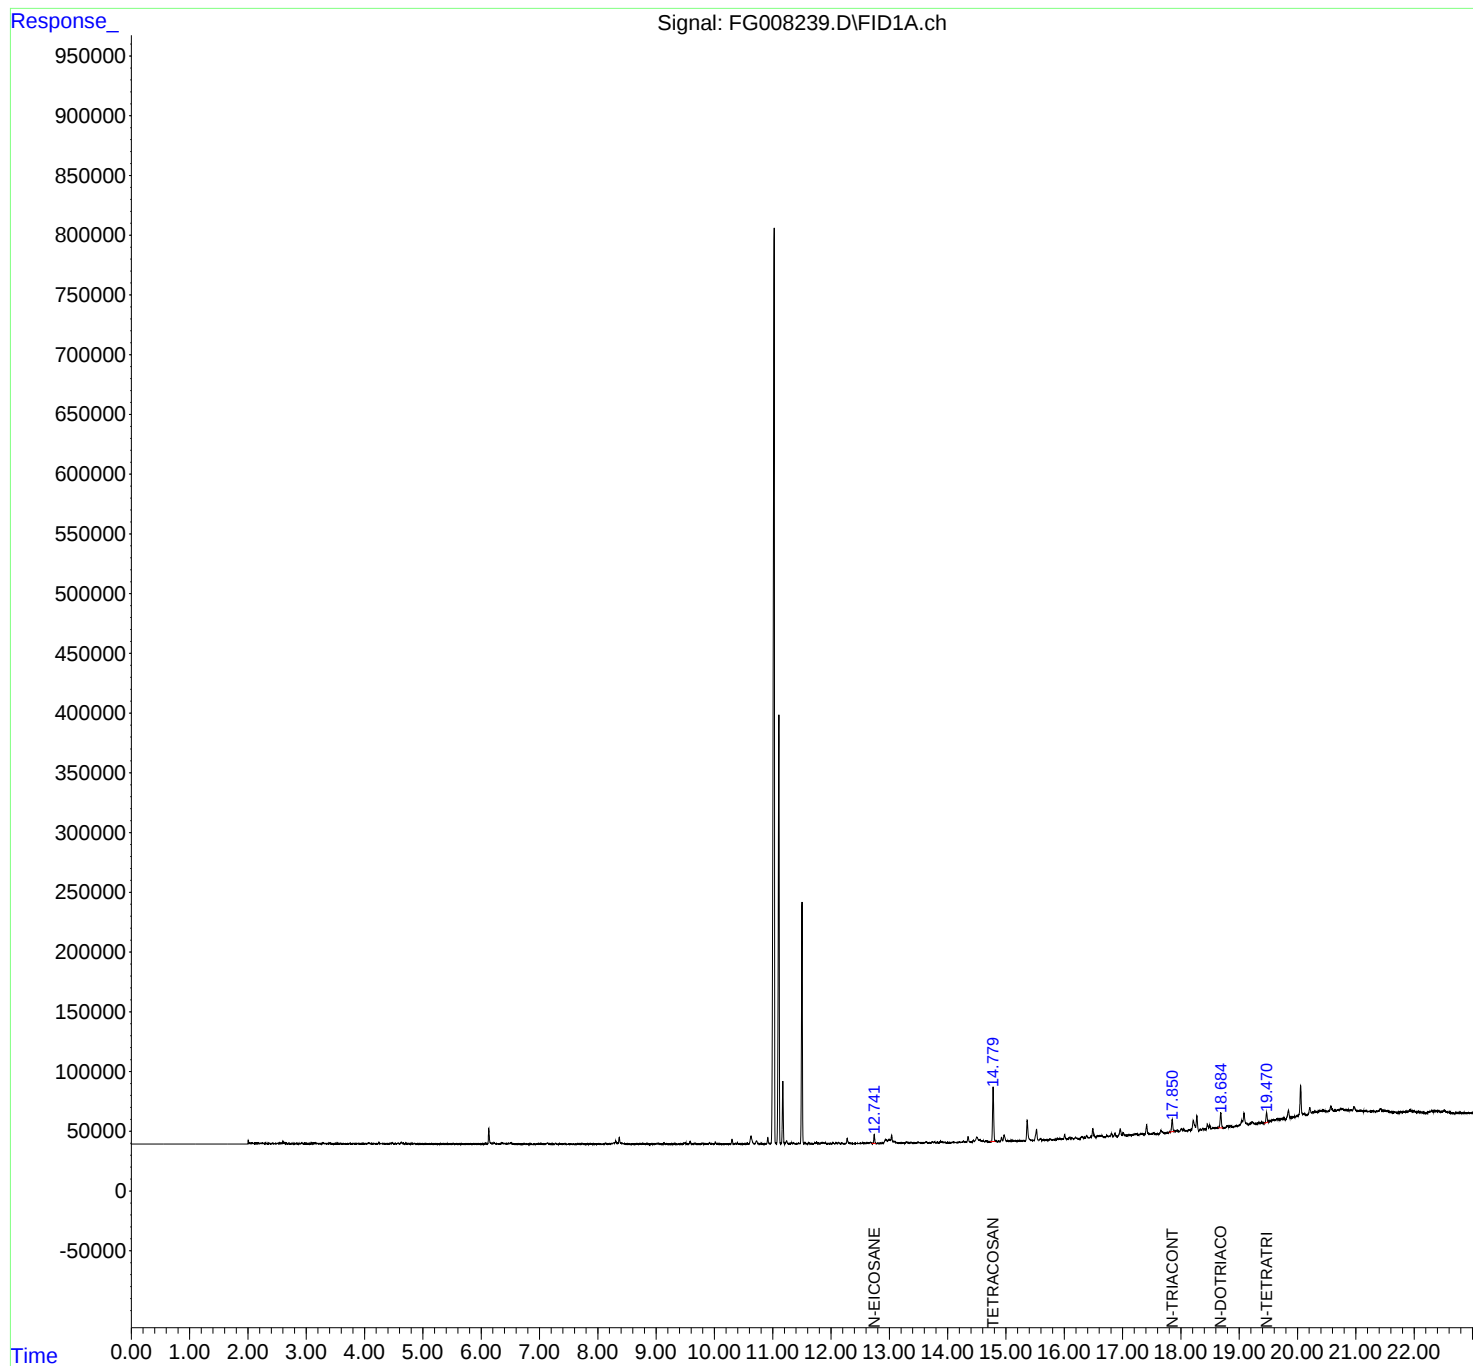


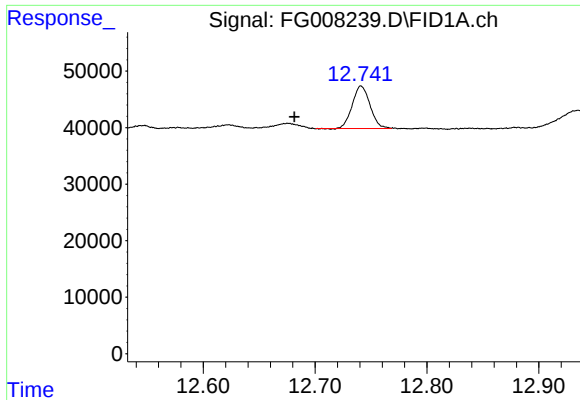

#7 N-EICOSANE


R.T.: 12.741 min
Delta R.T.: 0.060 min
Response: 82790
Conc: 0.60 ug/ml

Instrument :
FID_G
ClientSampleId :

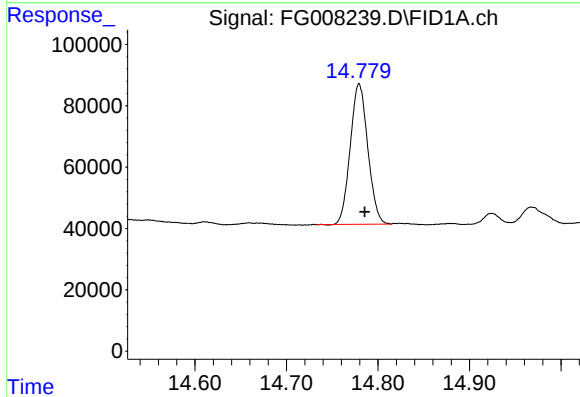


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.779 min
Delta R.T.: -0.006 min
Response: 609462
Conc: 5.14 ug/ml

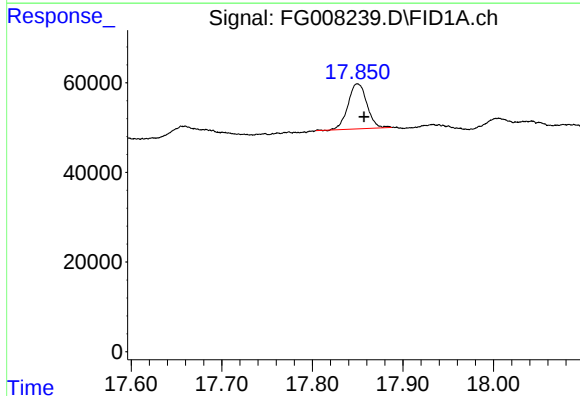


#13 N-TRIACONTANE

R.T.: 17.850 min
Delta R.T.: -0.007 min
Response: 145407
Conc: 1.14 ug/ml

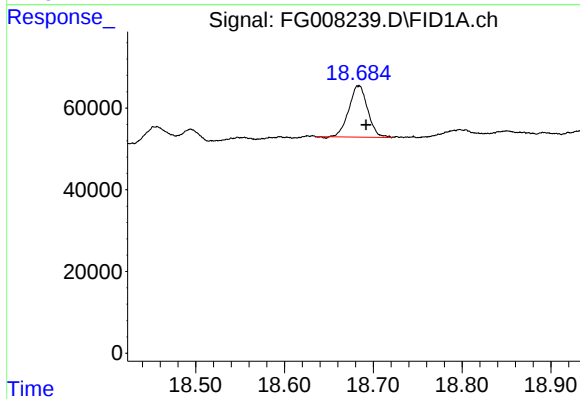

#14 N-DOTRIACONTANE

R.T.: 18.684 min
Delta R.T.: -0.008 min
Response: 185253
Conc: 1.49 ug/ml

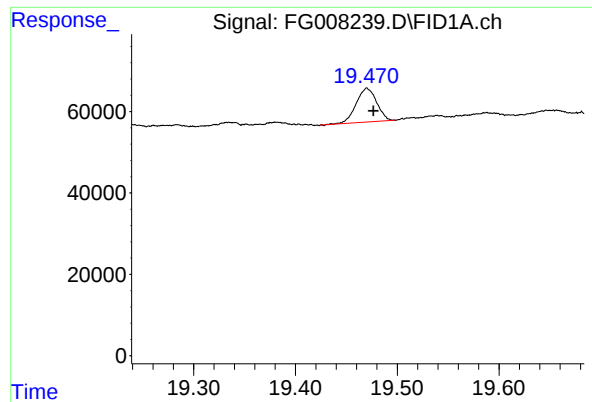

#15 N-TETRATRIACONTANE

R.T.: 19.470 min

Delta R.T.: -0.006 min

Response: 115995

Conc: 0.99 ug/ml

Instrument :
FID_G
ClientSampleId :