

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060721\
Data File : FG008240.D
Signal(s) : FID1A.ch
Acq On : 07 Jun 2021 19:52
Operator : DD\AJ
Sample : M2612-02 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 02:01:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	388889	3.277 ug/ml
Target Compounds			
4) N-TETRADECANE	8.368f	135981	0.997 ug/ml
7) N-EICOSANE	12.740f	519198	3.793 ug/ml
10) N-TETRACOSANE	14.966	279667	2.079 ug/ml
12) N-OCTACOSANE	16.968	77012	0.594 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060721\
Data File : FG008240.D
Signal(s) : FID1A.ch
Acq On : 07 Jun 2021 19:52
Operator : DD\AJ
Sample : M2612-02 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 02:01:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

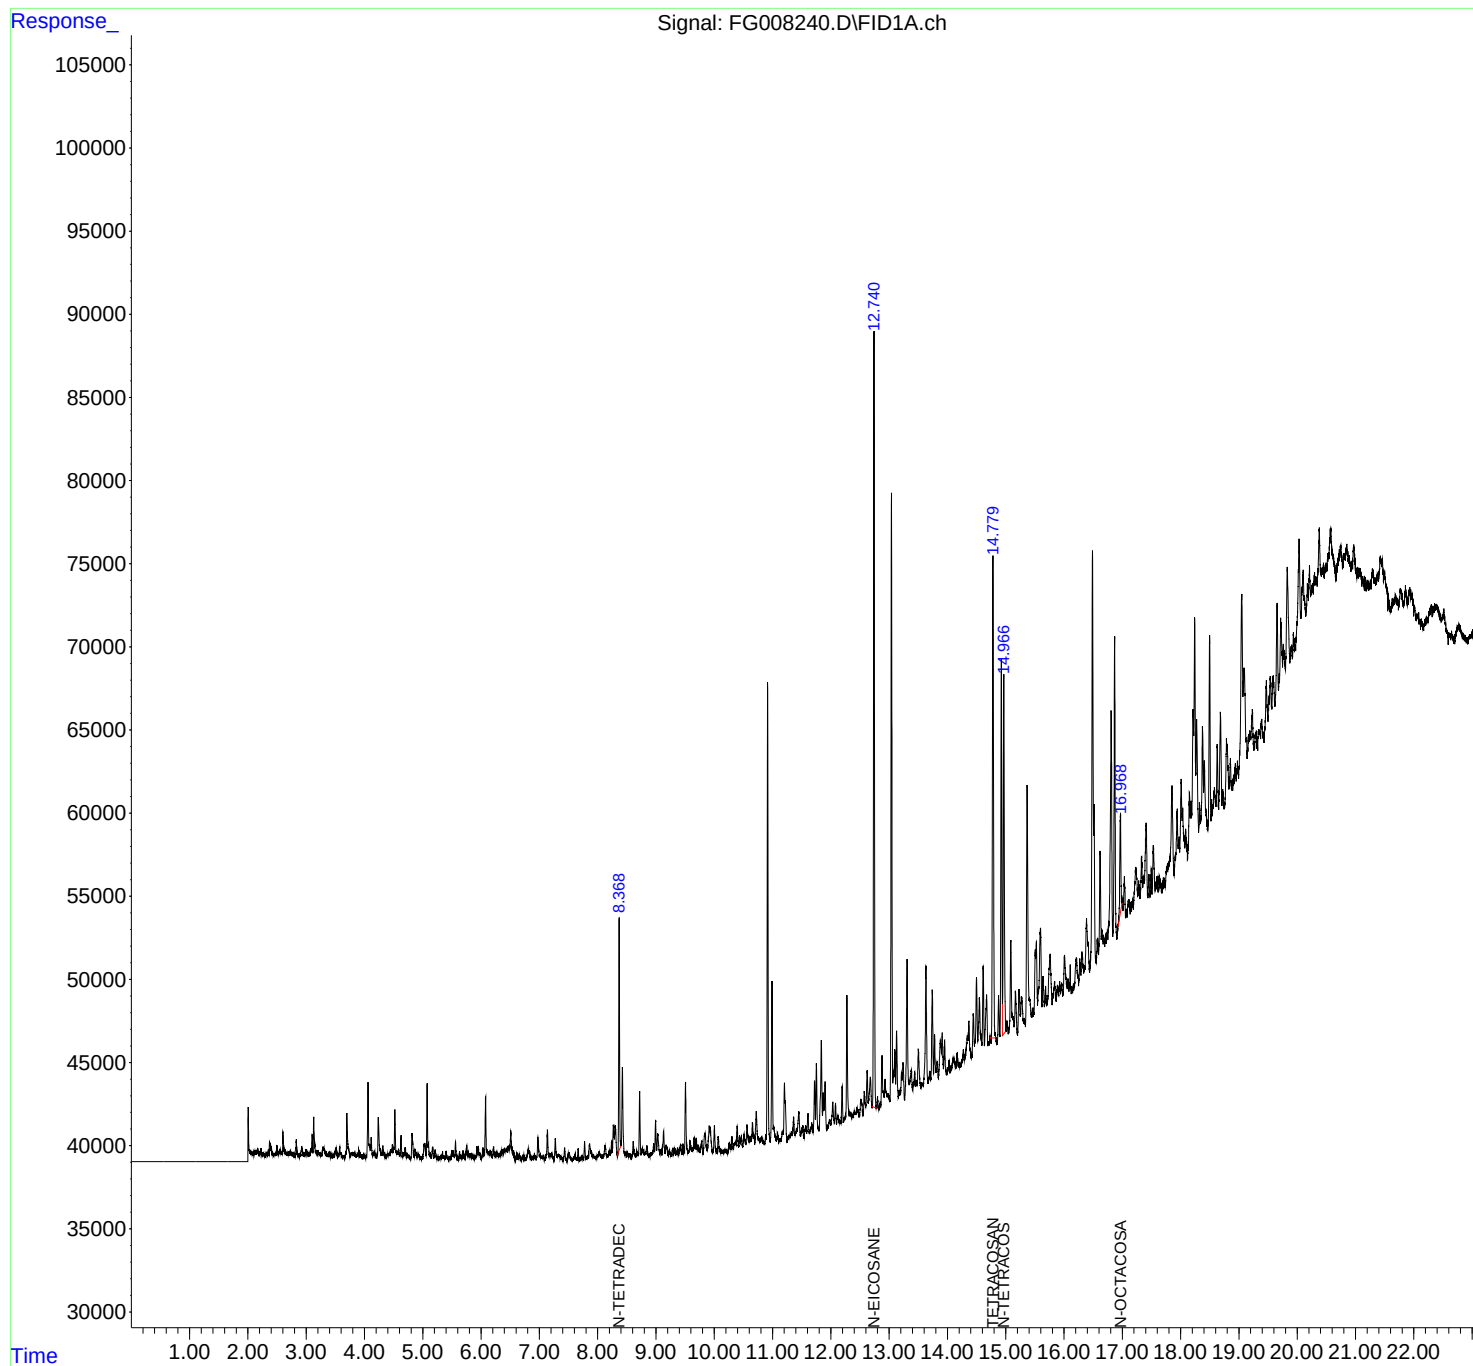


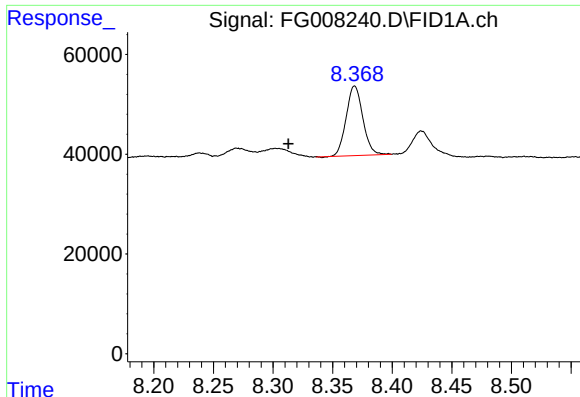

#4 N-TETRADECANE


R.T.: 8.368 min
Delta R.T.: 0.056 min
Response: 135981
Conc: 1.00 ug/ml

Instrument :
FID_G
ClientSampleId :

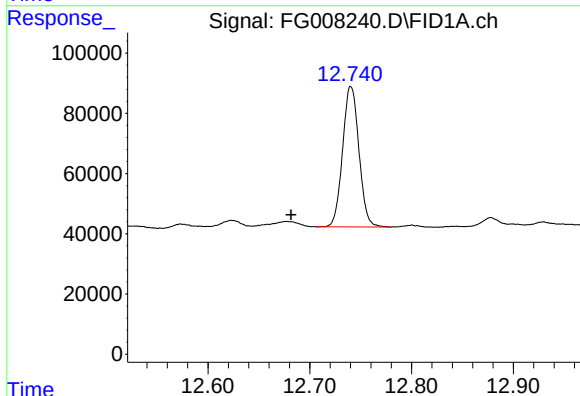


#7 N-EICOSANE

R.T.: 12.740 min
Delta R.T.: 0.059 min
Response: 519198
Conc: 3.79 ug/ml

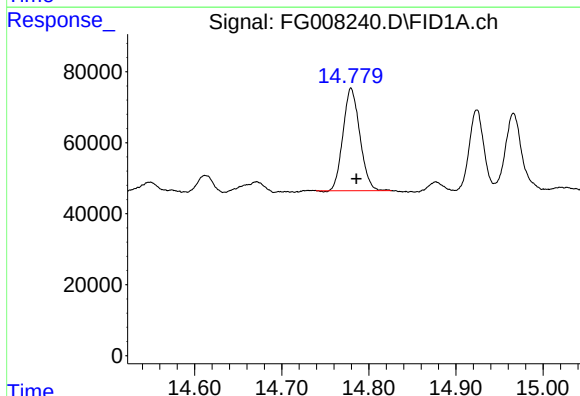


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: -0.006 min
Response: 388889
Conc: 3.28 ug/ml

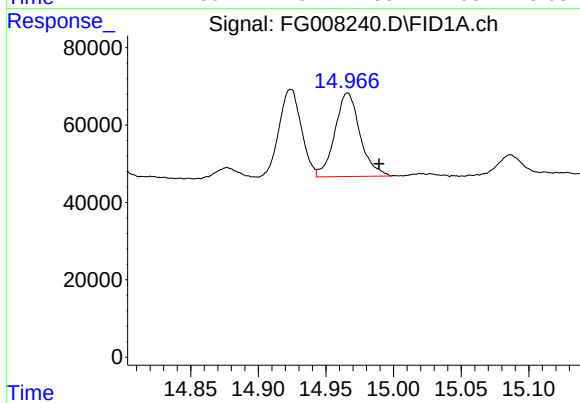

#10 N-TETRACOSANE

R.T.: 14.966 min
Delta R.T.: -0.023 min
Response: 279667
Conc: 2.08 ug/ml

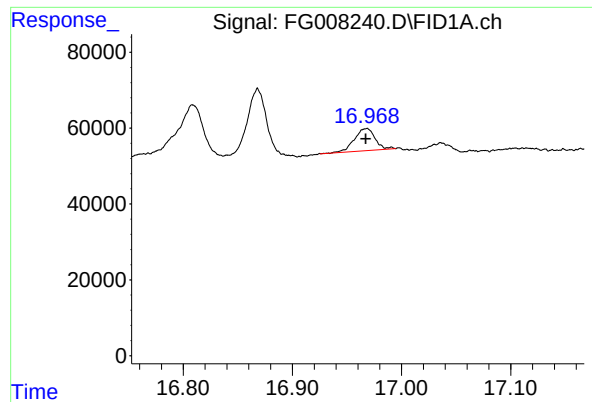

#12 N-OCTACOSANE

R.T.: 16.968 min
Delta R.T.: 0.000 min
Response: 77012
Conc: 0.59 ug/ml

Instrument :
FID_G
ClientSampleId :