

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060721\
 Data File : FG008226.D
 Signal(s) : FID1A.ch
 Acq On : 07 Jun 2021 11:58
 Operator : DD\AJ
 Sample : M2612-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 18-B12(70-74)

Integration File: autoint1.e
 Quant Time: Jun 08 01:59:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.782	2110454	17.784 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060721\
Data File : FG008226.D
Signal(s) : FID1A.ch
Acq On : 07 Jun 2021 11:58
Operator : DD\AJ
Sample : M2612-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
18-B12(70-74)

Integration File: autoint1.e
Quant Time: Jun 08 01:59:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

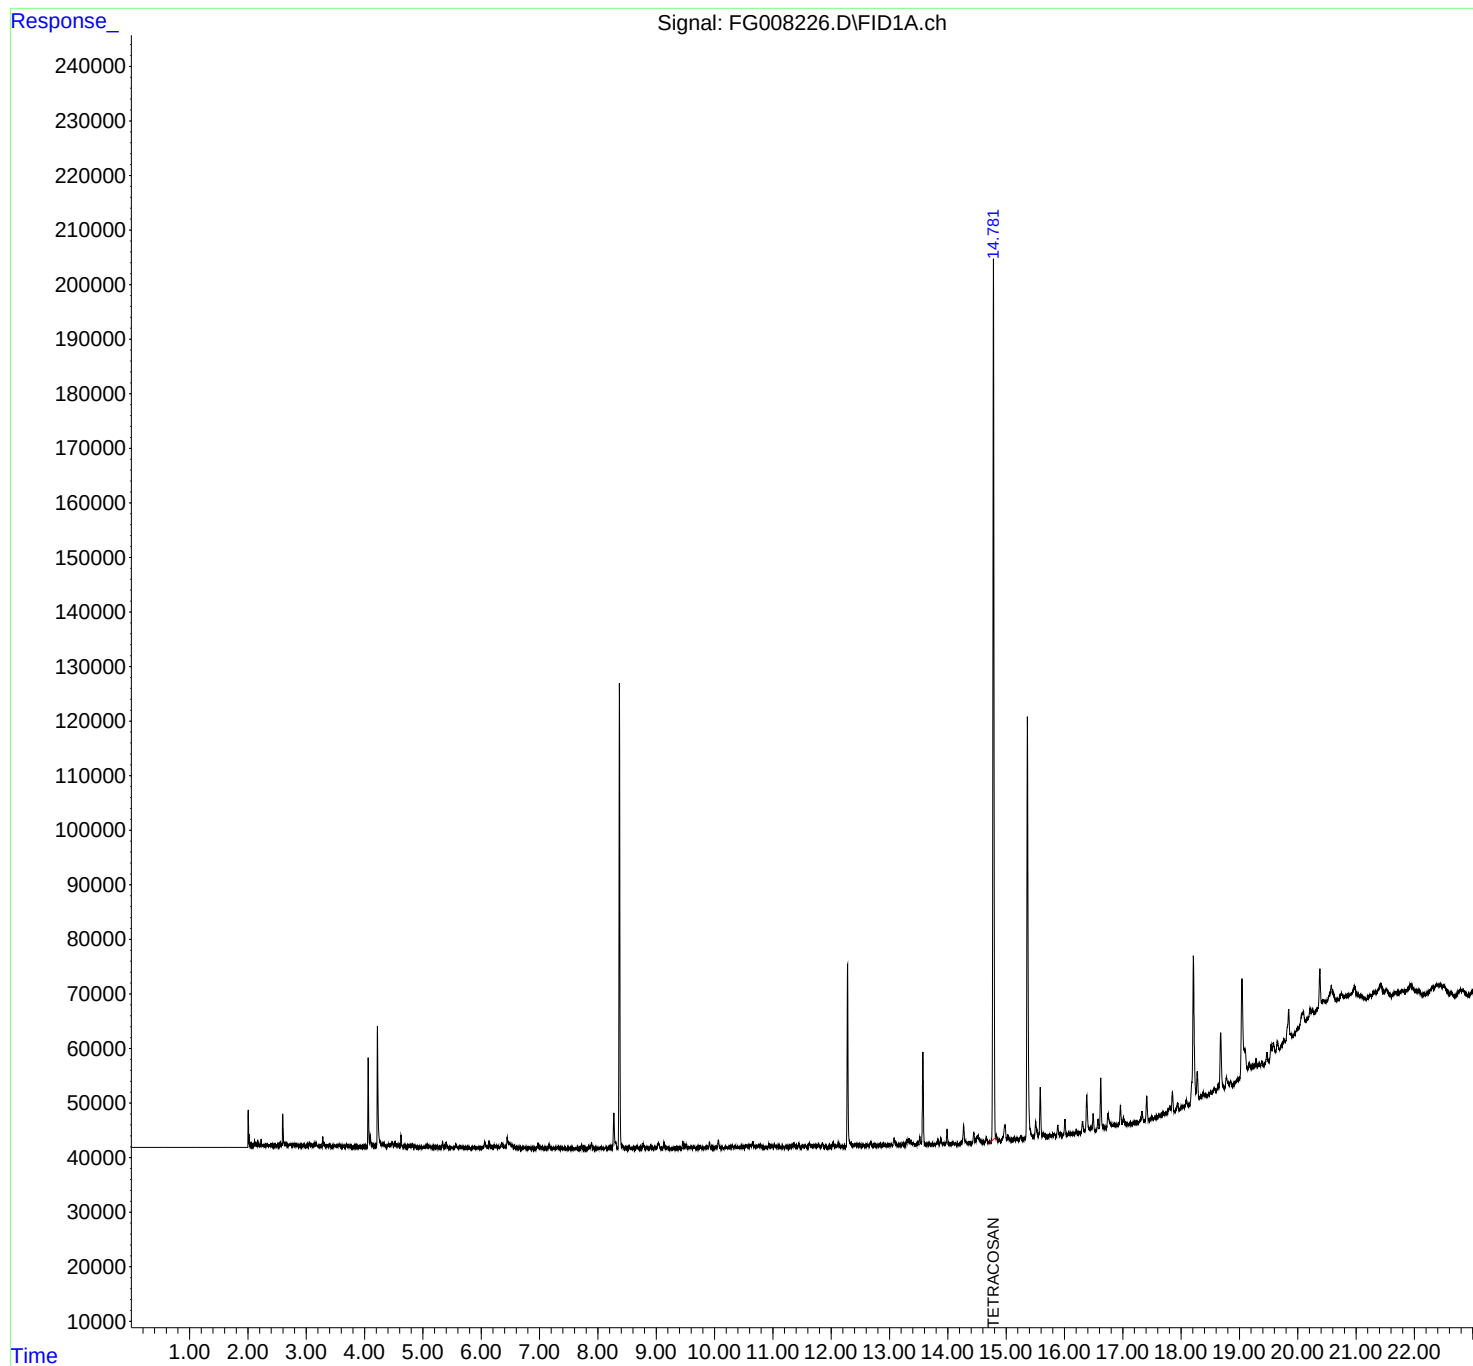

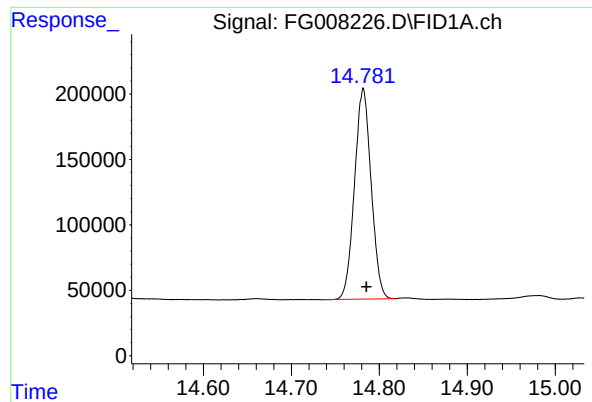

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.782 min
Delta R.T.: -0.004 min
Response: 2110454
Conc: 17.78 ug/ml

Instrument :
FID_G
ClientSampleId :
18-B12(70-74)