

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060721\
 Data File : FG008240.D
 Signal(s) : FID1A.ch
 Acq On : 07 Jun 2021 19:52
 Operator : DD\AJ
 Sample : M2612-02 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 18-B12(10-14)

Integration File: autoint1.e
 Quant Time: Jun 08 02:01:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	388889	3.277 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060721\
Data File : FG008240.D
Signal(s) : FID1A.ch
Acq On : 07 Jun 2021 19:52
Operator : DD\AJ
Sample : M2612-02 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
18-B12(10-14)

Integration File: autoint1.e
Quant Time: Jun 08 02:01:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

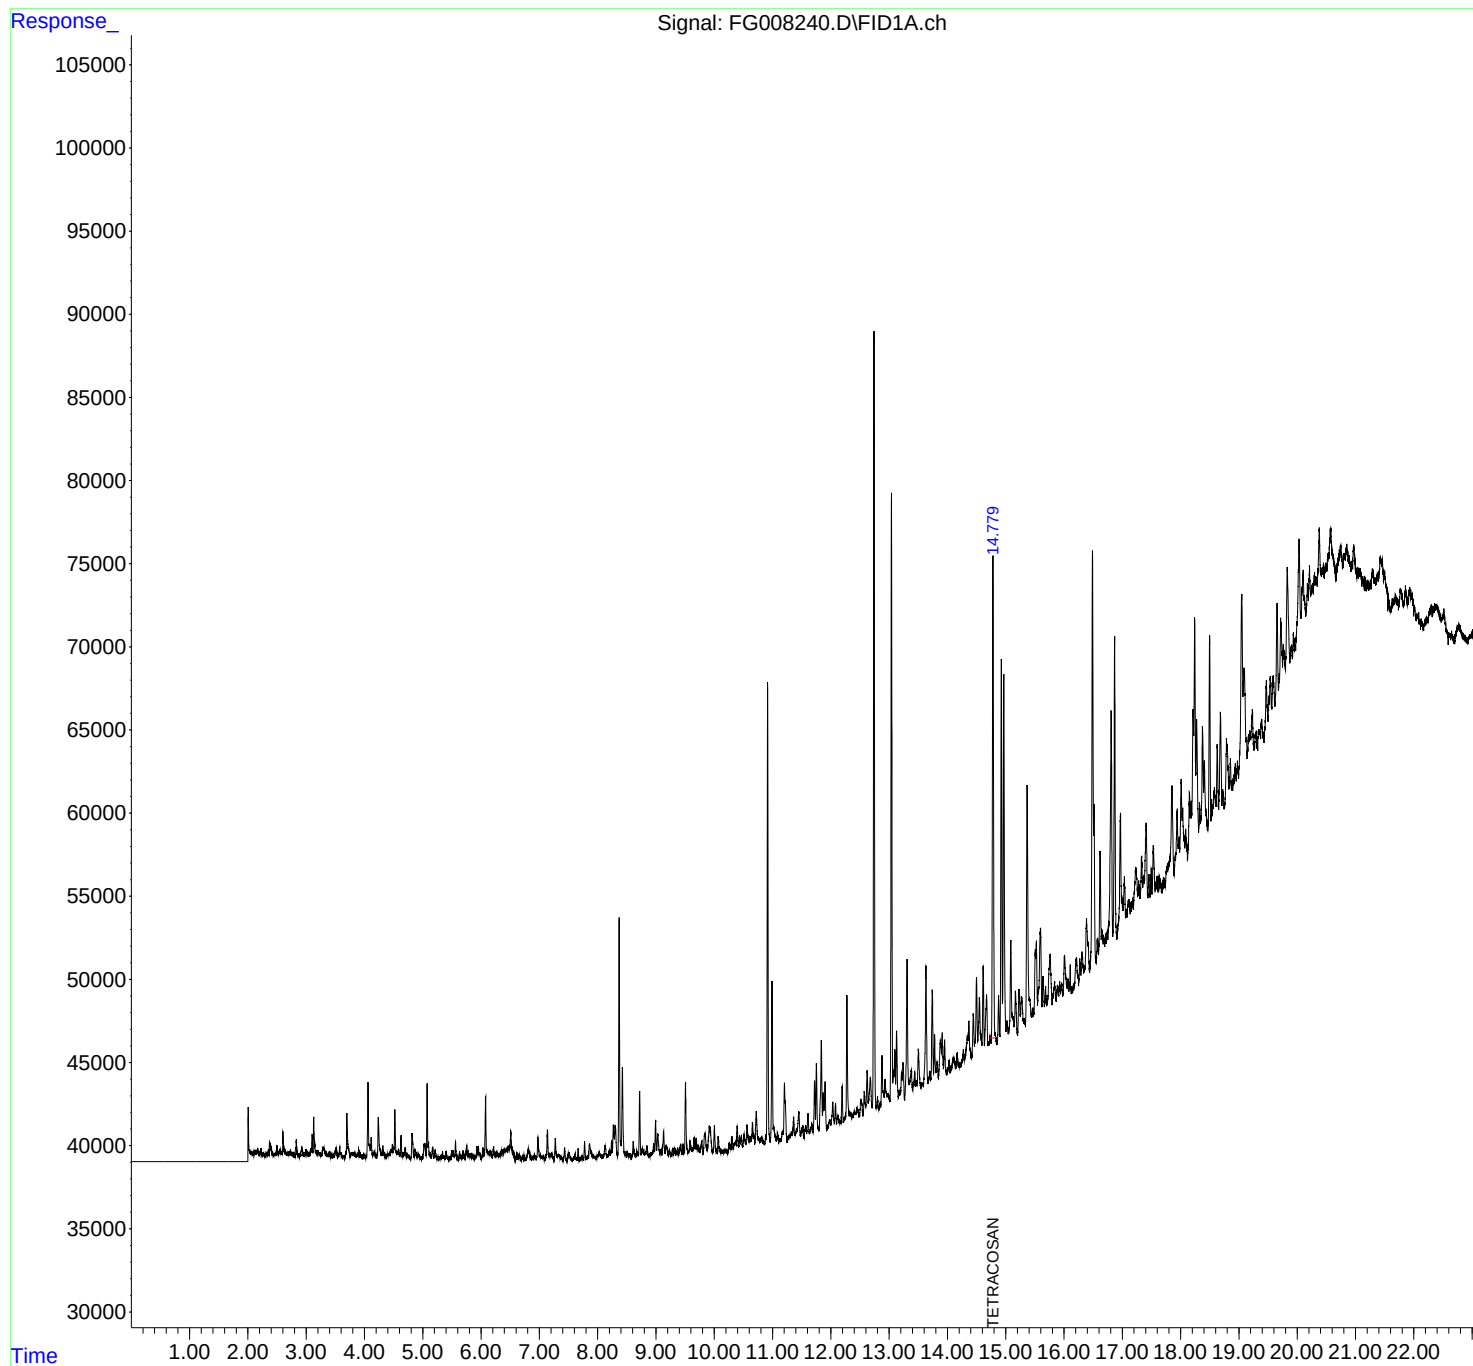

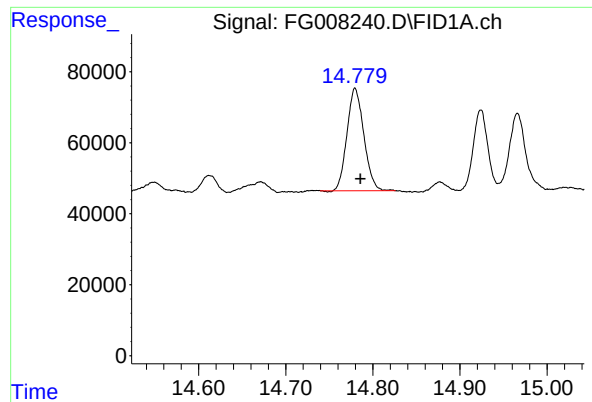

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: -0.006 min
Response: 388889
Conc: 3.28 ug/ml

Instrument :
FID_G
ClientSampleId :
18-B12(10-14)