

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG060821\  
Data File : FG008251.D  
Signal(s) : FID1A.ch  
Acq On : 08 Jun 2021 16:14  
Operator : DD\AJ  
Sample : M2637-05  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jun 09 01:09:35 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052521.M  
Quant Title :  
QLast Update : Wed May 26 08:20:50 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

|                             | Compound                 | R.T.   | Response | Conc Units   |
|-----------------------------|--------------------------|--------|----------|--------------|
| -----                       |                          |        |          |              |
| System Monitoring Compounds |                          |        |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.779 | 1782269  | 15.018 ug/ml |
|                             |                          |        |          |              |
| Target Compounds            |                          |        |          |              |
| 12)                         | N-OCTACOSANE             | 17.009 | 150034   | 1.158 ug/ml  |
| -----                       |                          |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG060821\  
Data File : FG008251.D  
Signal(s) : FID1A.ch  
Acq On : 08 Jun 2021 16:14  
Operator : DD\AJ  
Sample : M2637-05  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jun 09 01:09:35 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052521.M  
Quant Title :  
QLast Update : Wed May 26 08:20:50 2021  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

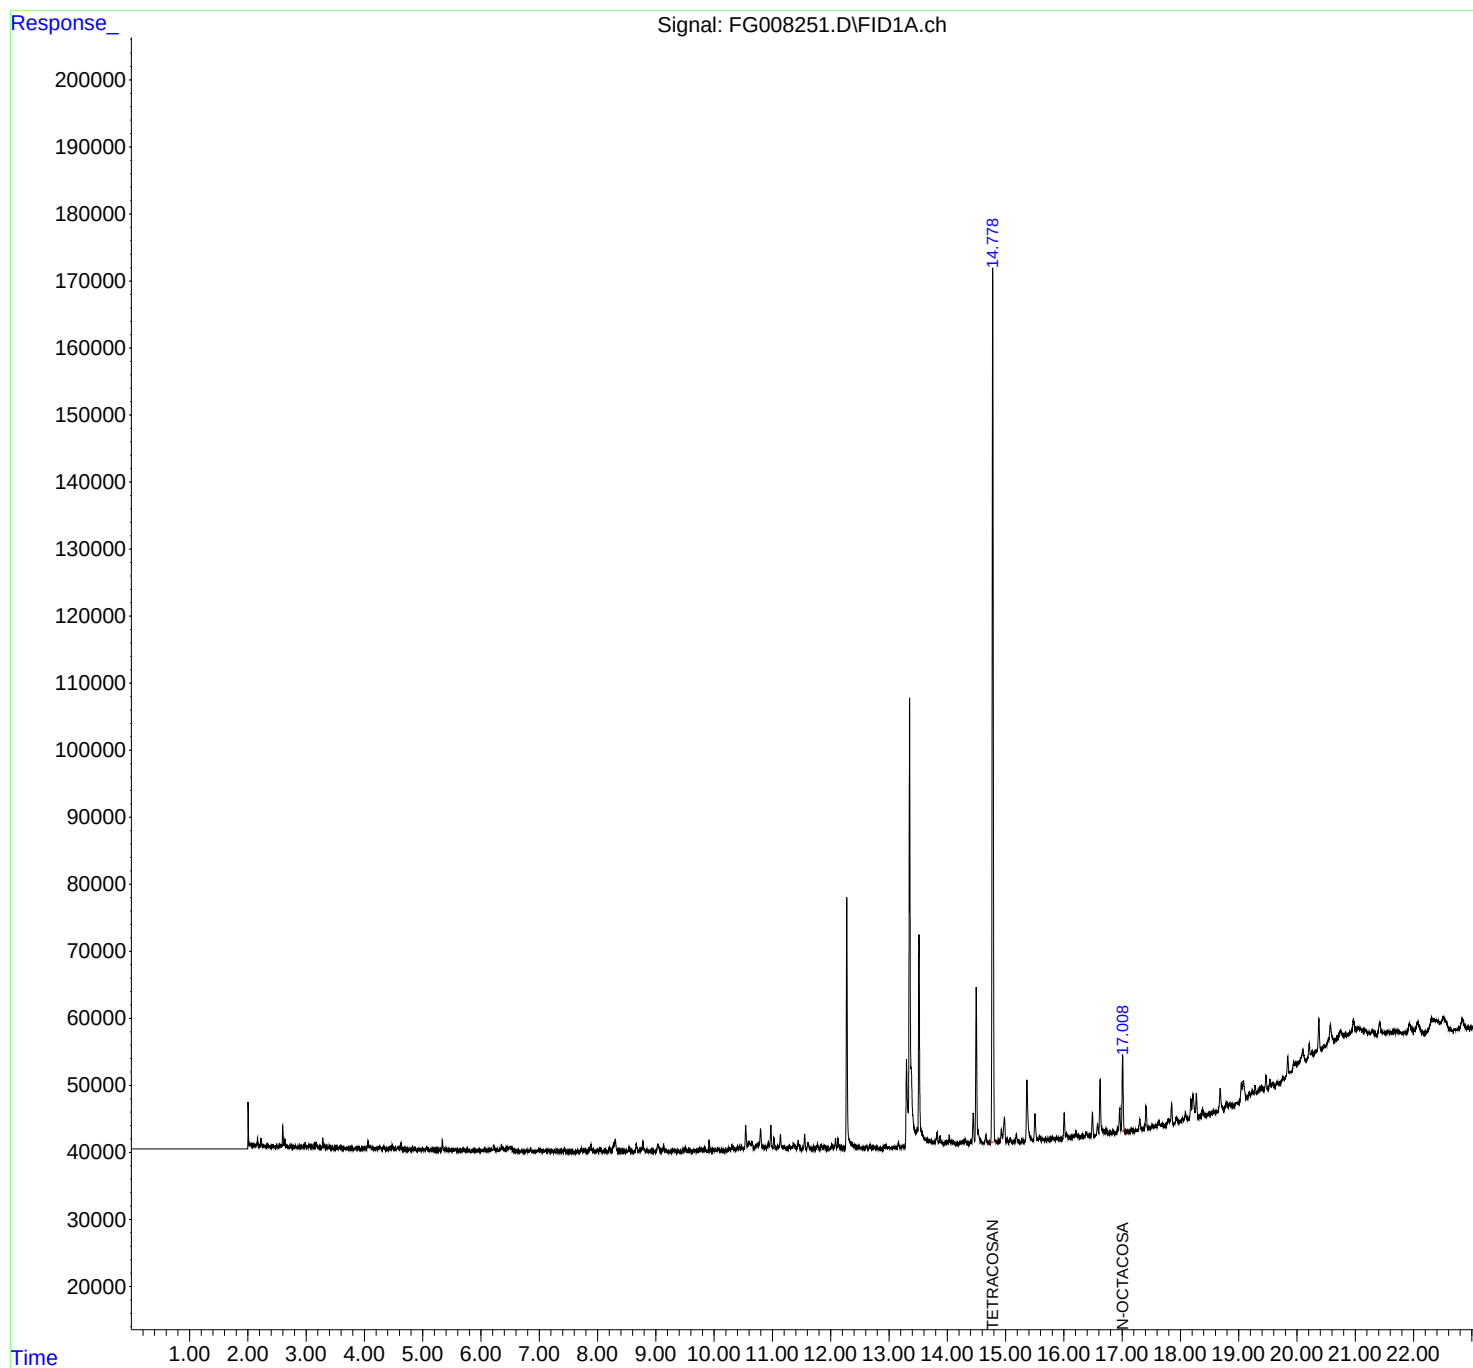

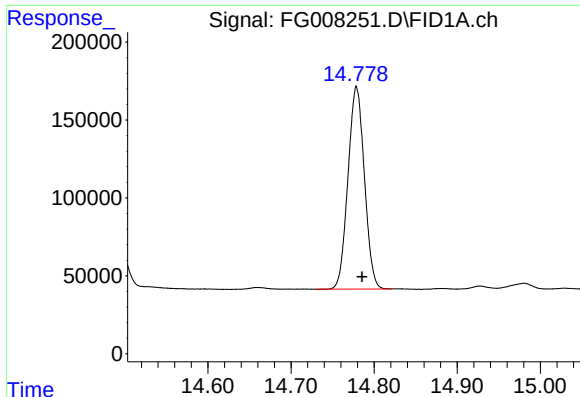

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.779 min  
Delta R.T.: -0.007 min  
Response: 1782269  
Conc: 15.02 ug/ml

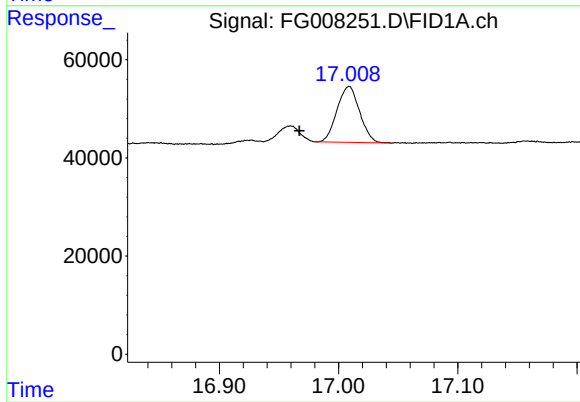

#12 N-OCTACOSANE

R.T.: 17.009 min  
Delta R.T.: 0.042 min  
Response: 150034  
Conc: 1.16 ug/ml