

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060822\
Data File : FG009834.D
Signal(s) : FID1A.ch
Acq On : 08 Jun 2022 11:49
Operator : AJ\MA
Sample : PB143273BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB143273BL

Integration File: autoint1.e
Quant Time: Jun 09 02:06:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.837	1902342	18.073 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060822\
Data File : FG009834.D
Signal(s) : FID1A.ch
Acq On : 08 Jun 2022 11:49
Operator : AJ\MA
Sample : PB143273BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB143273BL

Integration File: autoint1.e
Quant Time: Jun 09 02:06:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

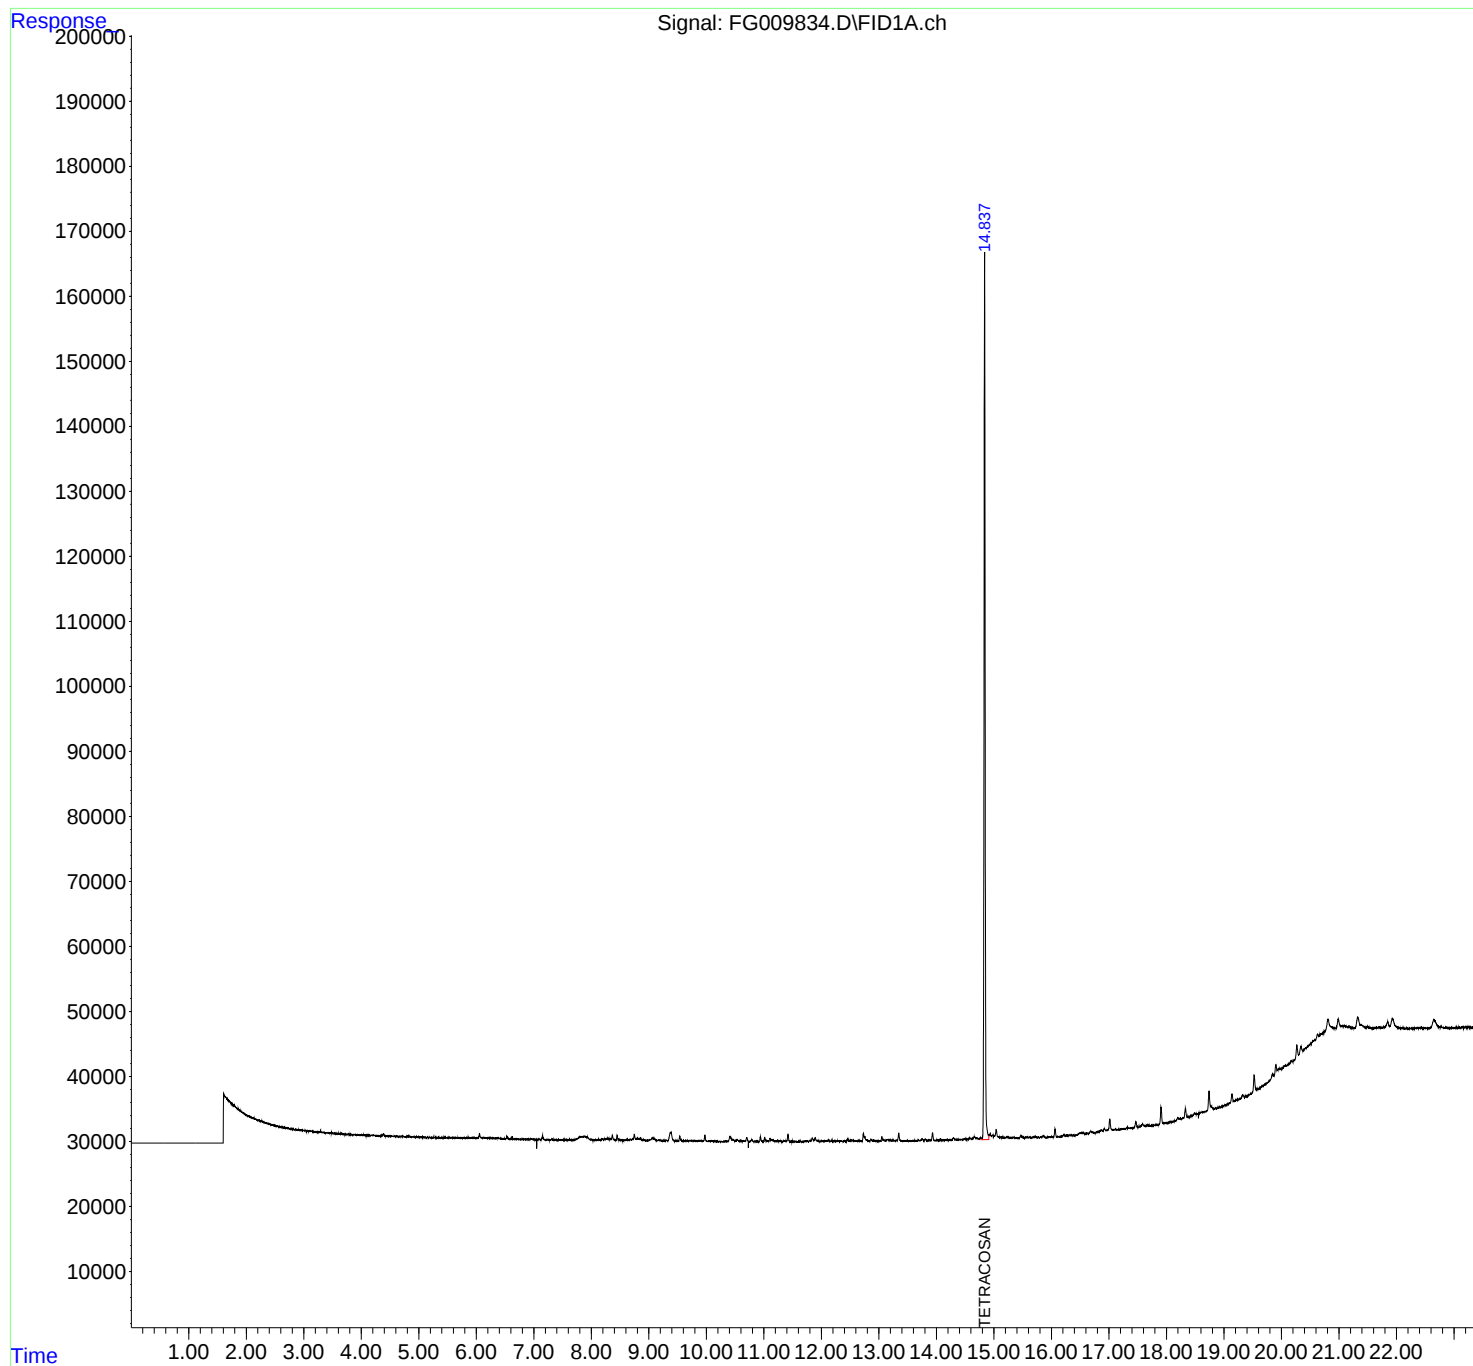

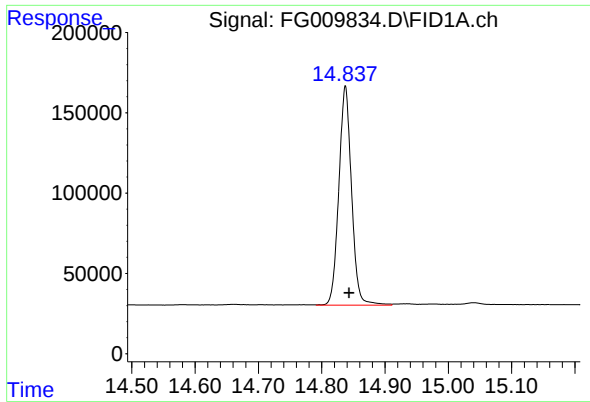

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.837 min
Delta R.T.: -0.006 min
Response: 1902342
Conc: 18.07 ug/ml

Instrument :
FID_G
ClientSampleId :
PB143273BL