

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060920\
Data File : FG006962.D
Signal(s) : FID1A.ch
Acq On : 09 Jun 2020 12:37
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 10 02:22:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG051520.M
Quant Title :
QLast Update : Sat May 16 01:41:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.518	4862461	34.218 ug/ml
12)	N-OCTACOSANE	16.962	4328904	30.333 ug/ml
13)	N-TRIACONTANE	17.849	302281	2.099 ug/ml
14)	N-DOTRIACONTANE	18.681	330374	2.392 ug/ml
15)	N-TETRATRIACONTANE	19.468	253510	1.939 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060920\
Data File : FG006962.D
Signal(s) : FID1A.ch
Acq On : 09 Jun 2020 12:37
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 10 02:22:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG051520.M
Quant Title :
QLast Update : Sat May 16 01:41:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

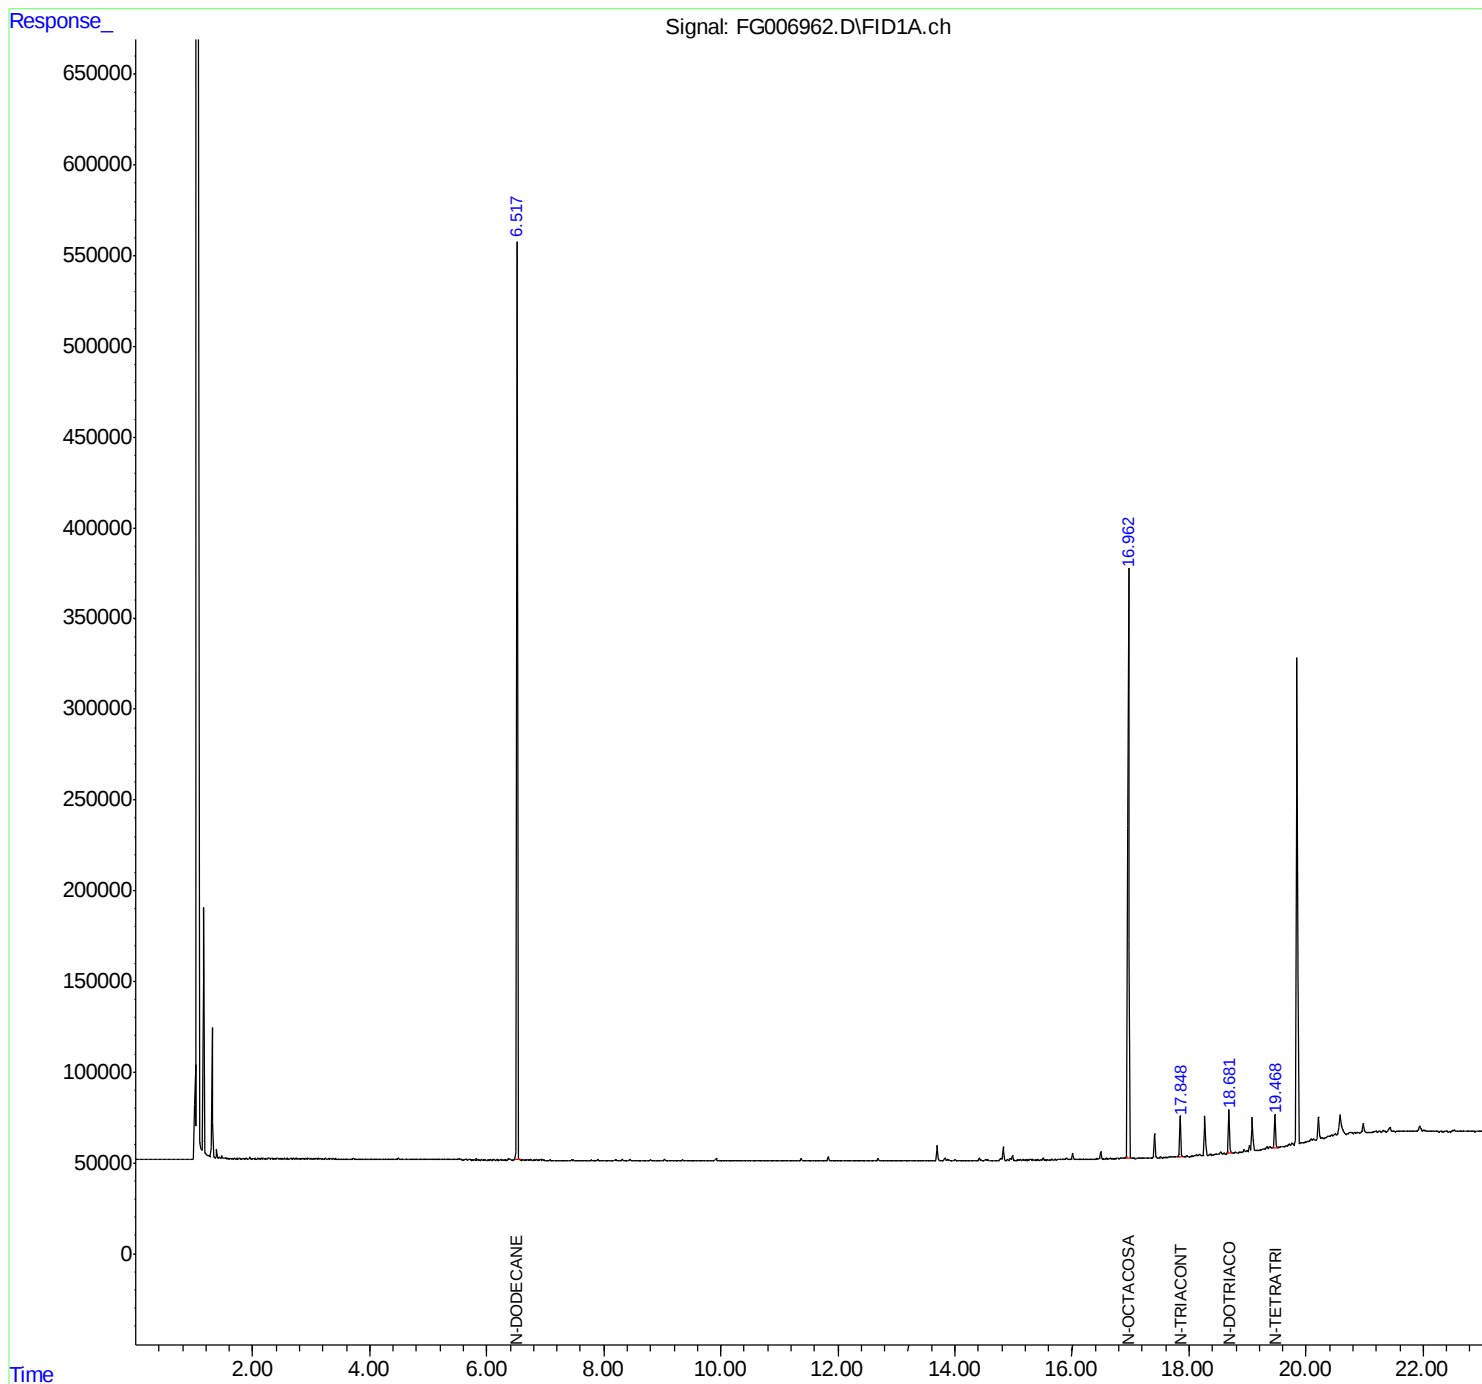


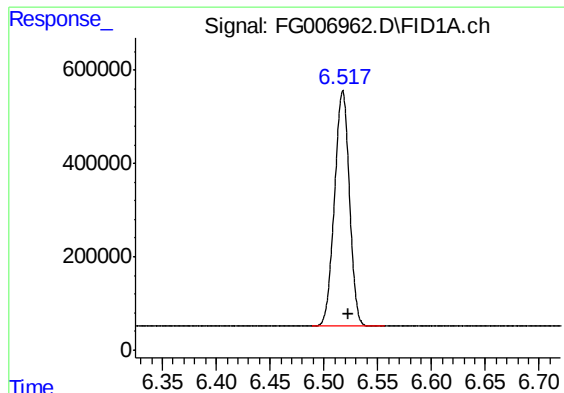

#3 N-DODECANE


R.T.: 6.518 min
Delta R.T.: -0.005 min
Response: 4862461
Conc: 34.22 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

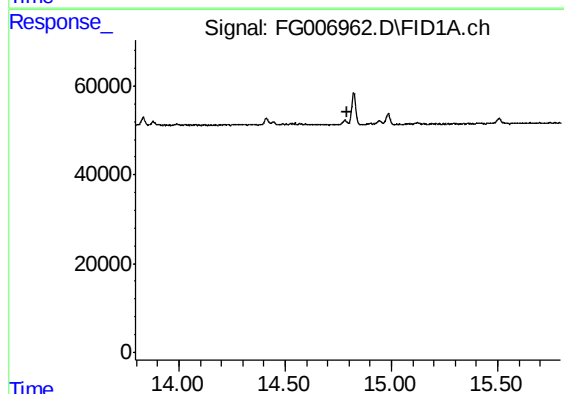


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.795 min
Response: 0
Conc: N.D.

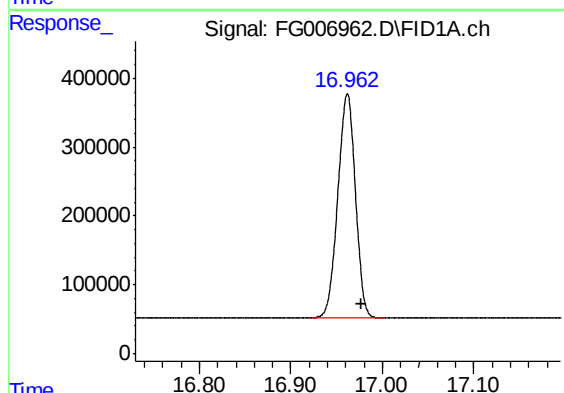


#12 N-OCTACOSANE

R.T.: 16.962 min
Delta R.T.: -0.016 min
Response: 4328904
Conc: 30.33 ug/ml

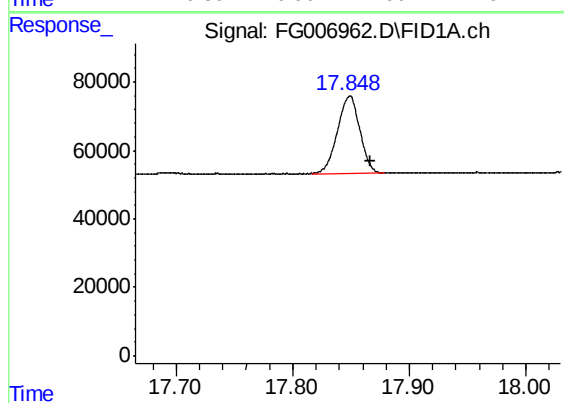

#13 N-TRIACONTANE


R.T.: 17.849 min
Delta R.T.: -0.018 min
Response: 302281
Conc: 2.10 ug/ml

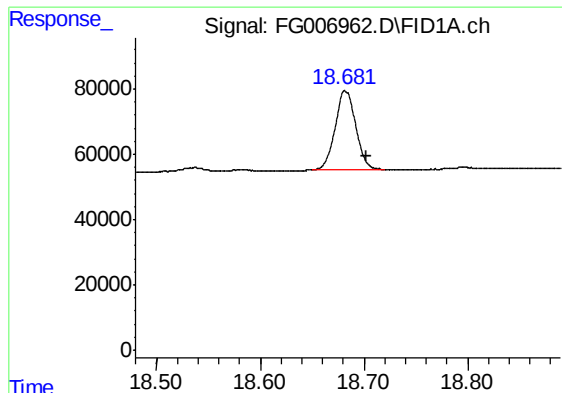

#14 N-DOTRIACONTANE

R.T.: 18.681 min
Delta R.T.: -0.021 min
Response: 330374
Conc: 2.39 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

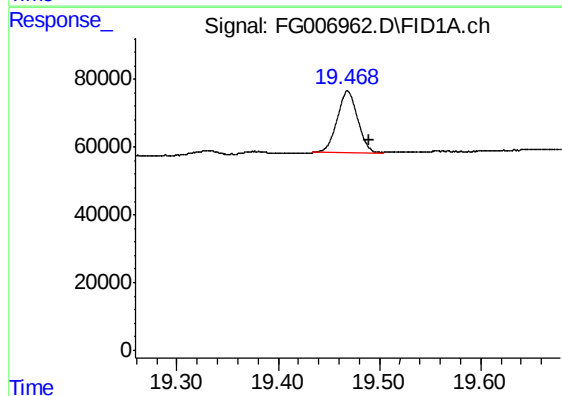

#15 N-TETRATRIACONTANE

R.T.: 19.468 min
Delta R.T.: -0.022 min
Response: 253510
Conc: 1.94 ug/ml