

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060920\
 Data File : FG060920.D
 Signal(s) : FID1A.ch
 Acq On : 09 Jun 2020 14:15
 Operator : DD\AJ
 Sample : L2936-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 WASTE

Integration File: autoint1.e
 Quant Time: Jun 10 02:22:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG051520.M
 Quant Title :
 QLast Update : Sat May 16 01:41:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	3151755	25.189 ug/ml
Target Compounds			
4) N-TETRADECANE	8.379f	1931481	13.456 ug/ml
7) N-EICOSANE	12.738	255305	1.780 ug/ml
10) N-TETRACOSANE	14.955	141690	0.990 ug/ml
11) N-HEXACOSANE	16.011	434058	3.047 ug/ml
12) N-OCTACOSANE	16.987	263925	1.849 ug/ml
13) N-TRIACONTANE	17.850	481961	3.347 ug/ml
14) N-DOTRIACONTANE	18.683	548702	3.973 ug/ml
15) N-TETRATRIACONTANE	19.536	361323	2.763 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060920\
Data File : FG006965.D
Signal(s) : FID1A.ch
Acq On : 09 Jun 2020 14:15
Operator : DD\AJ
Sample : L2936-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WASTE

Integration File: autoint1.e
Quant Time: Jun 10 02:22:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG051520.M
Quant Title :
QLast Update : Sat May 16 01:41:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

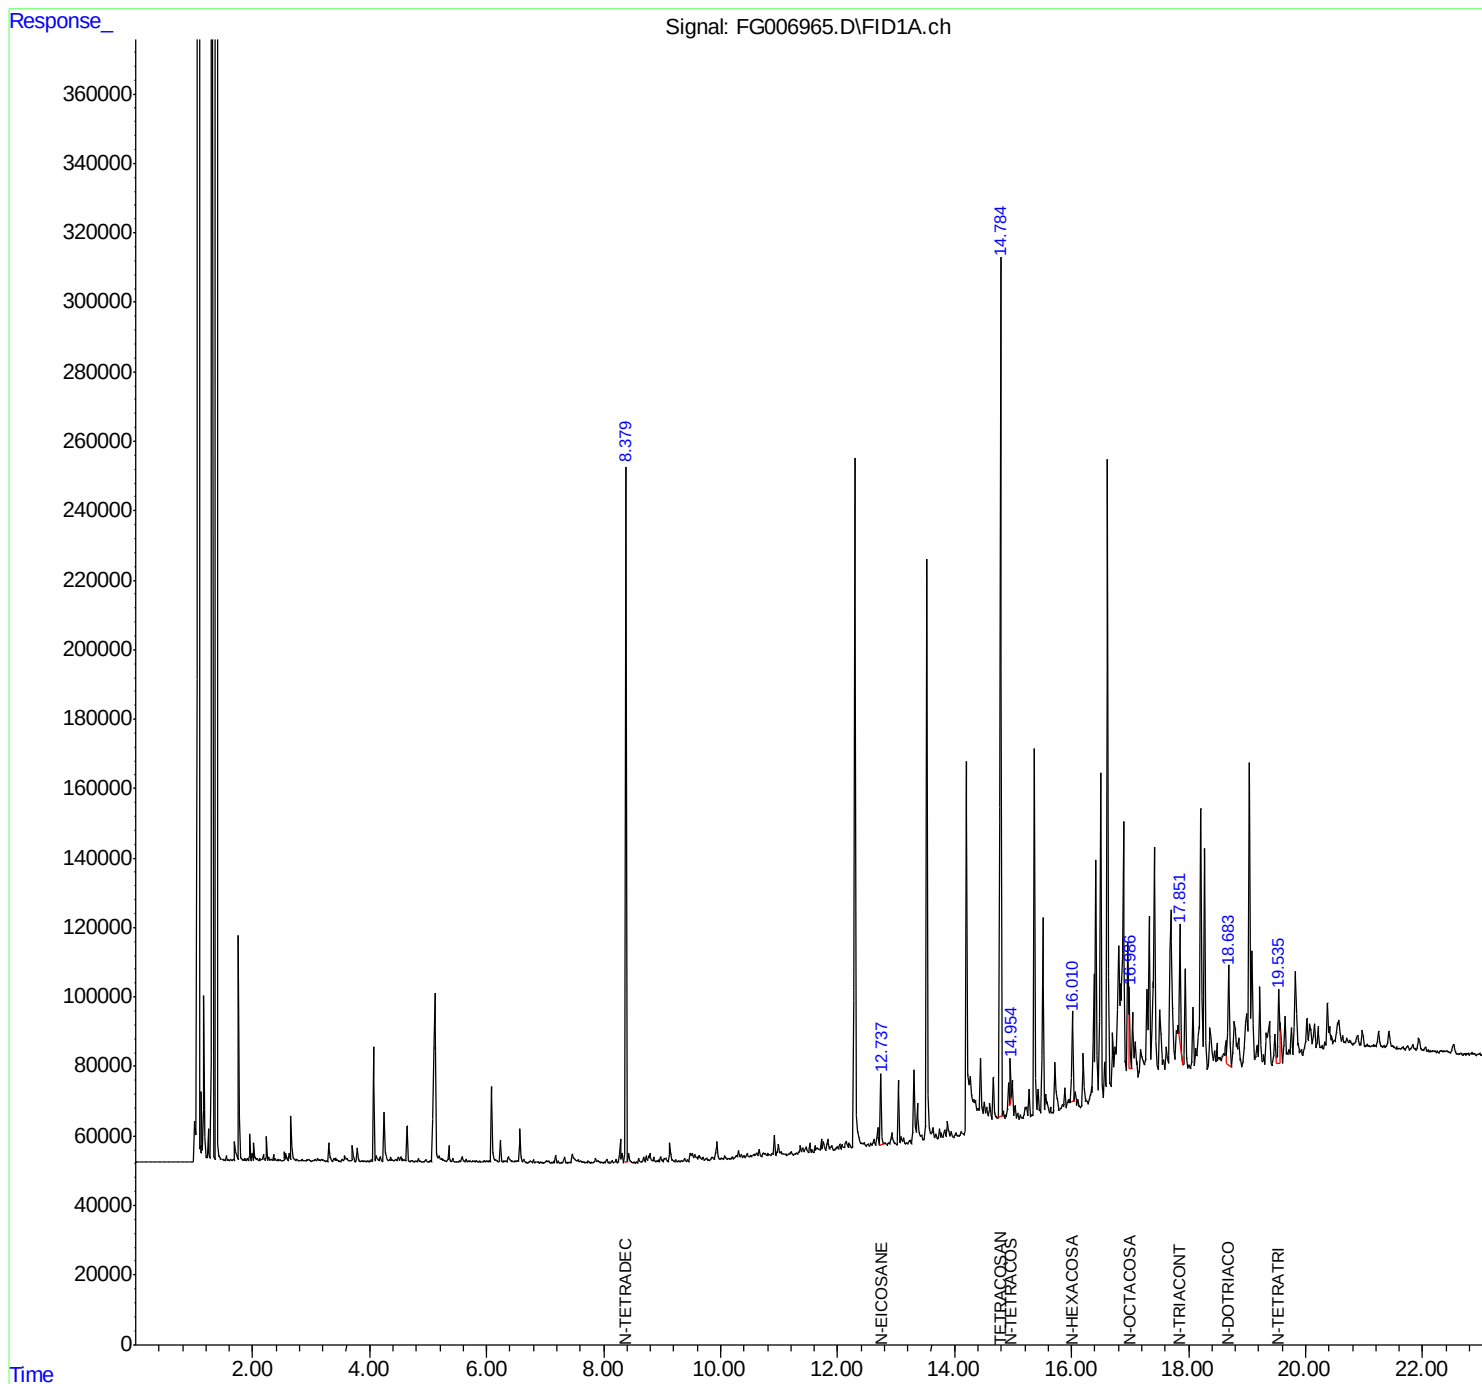


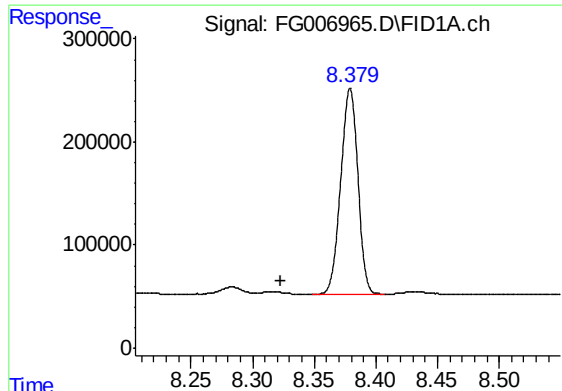

#4 N-TETRADECANE


R.T.: 8.379 min
Delta R.T.: 0.056 min
Response: 1931481
Conc: 13.46 ug/ml

Instrument :
FID_G
ClientSampleId :
WASTE

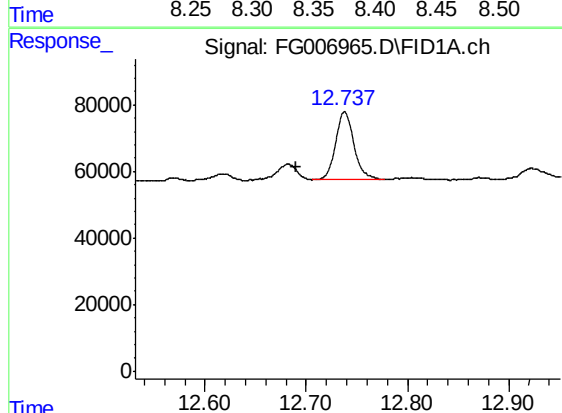


#7 N-EICOSANE

R.T.: 12.738 min
Delta R.T.: 0.048 min
Response: 255305
Conc: 1.78 ug/ml

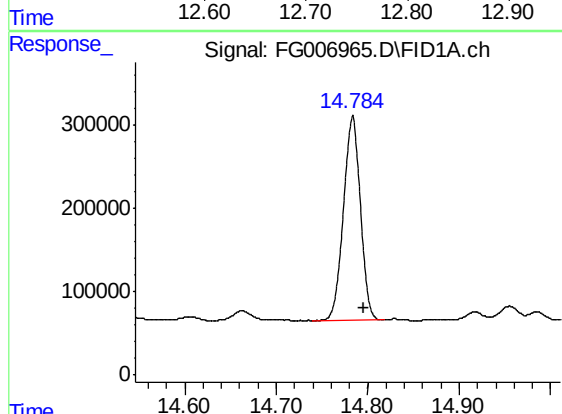


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.784 min
Delta R.T.: -0.012 min
Response: 3151755
Conc: 25.19 ug/ml

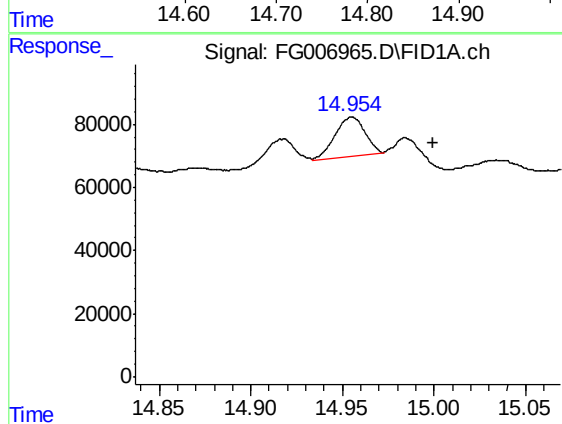

#10 N-TETRACOSANE


R.T.: 14.955 min
Delta R.T.: -0.045 min
Response: 141690
Conc: 0.99 ug/ml

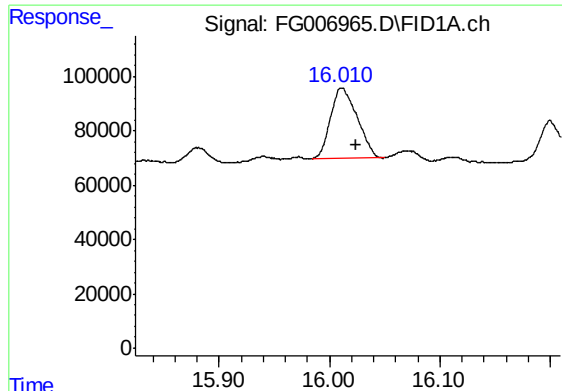

#11 N-HEXACOSANE


R.T.: 16.011 min
Delta R.T.: -0.014 min
Response: 434058
Conc: 3.05 ug/ml

Instrument :
FID_G
ClientSampleId :
WASTE

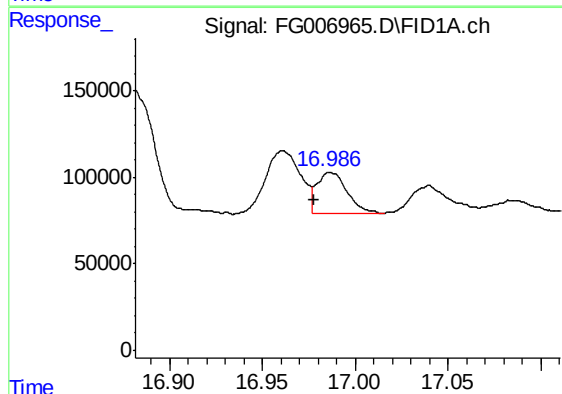


#12 N-OCTACOSANE

R.T.: 16.987 min
Delta R.T.: 0.009 min
Response: 263925
Conc: 1.85 ug/ml

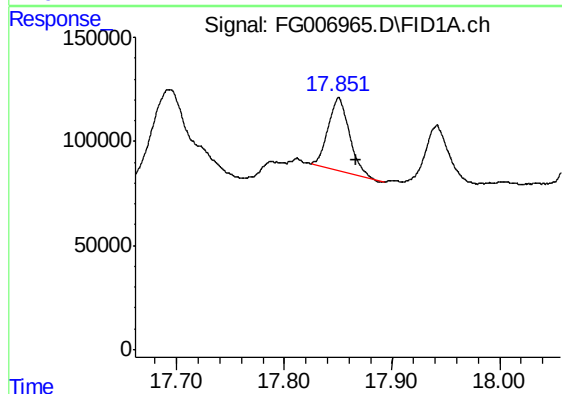


#13 N-TRIACONTANE

R.T.: 17.850 min
Delta R.T.: -0.016 min
Response: 481961
Conc: 3.35 ug/ml

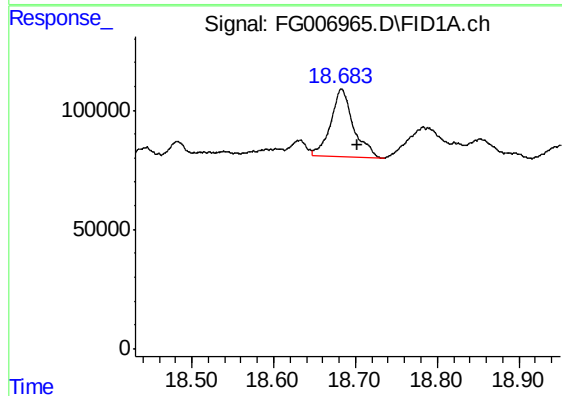

#14 N-DOTRIACONTANE

R.T.: 18.683 min
Delta R.T.: -0.020 min
Response: 548702
Conc: 3.97 ug/ml

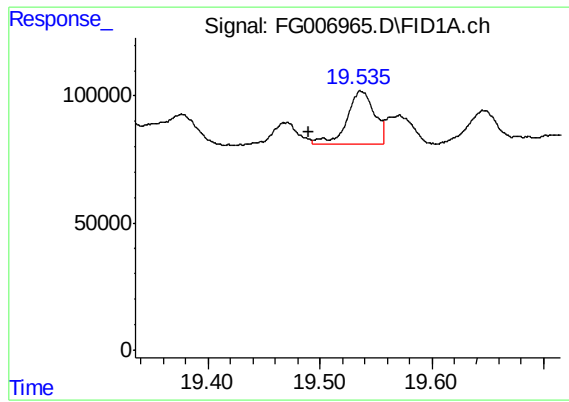

#15 N-TETRATRIACONTANE

R.T.: 19.536 min
Delta R.T.: 0.046 min
Response: 361323
Conc: 2.76 ug/ml

Instrument :
FID_G
ClientSampleId :
WASTE