

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG060921\  
 Data File : FG008263.D  
 Signal(s) : FID1A.ch  
 Acq On : 09 Jun 2021 20:09  
 Operator : DD\AJ  
 Sample : M2625-06  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jun 10 01:59:35 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052521.M  
 Quant Title :  
 QLast Update : Wed May 26 08:20:50 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units   |
|-------------------------------|---------|----------|--------------|
| -----                         |         |          |              |
| System Monitoring Compounds   |         |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.779  | 2212009  | 18.639 ug/ml |
| Target Compounds              |         |          |              |
| 13) N-TRIACONTANE             | 17.926f | 133603   | 1.047 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.675  | 166998   | 1.344 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.464  | 100578   | 0.860 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.211  | 57378    | 0.518 ug/ml  |
| -----                         |         |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG060921\  
Data File : FG008263.D  
Signal(s) : FID1A.ch  
Acq On : 09 Jun 2021 20:09  
Operator : DD\AJ  
Sample : M2625-06  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 10 01:59:35 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052521.M  
Quant Title :  
QLast Update : Wed May 26 08:20:50 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

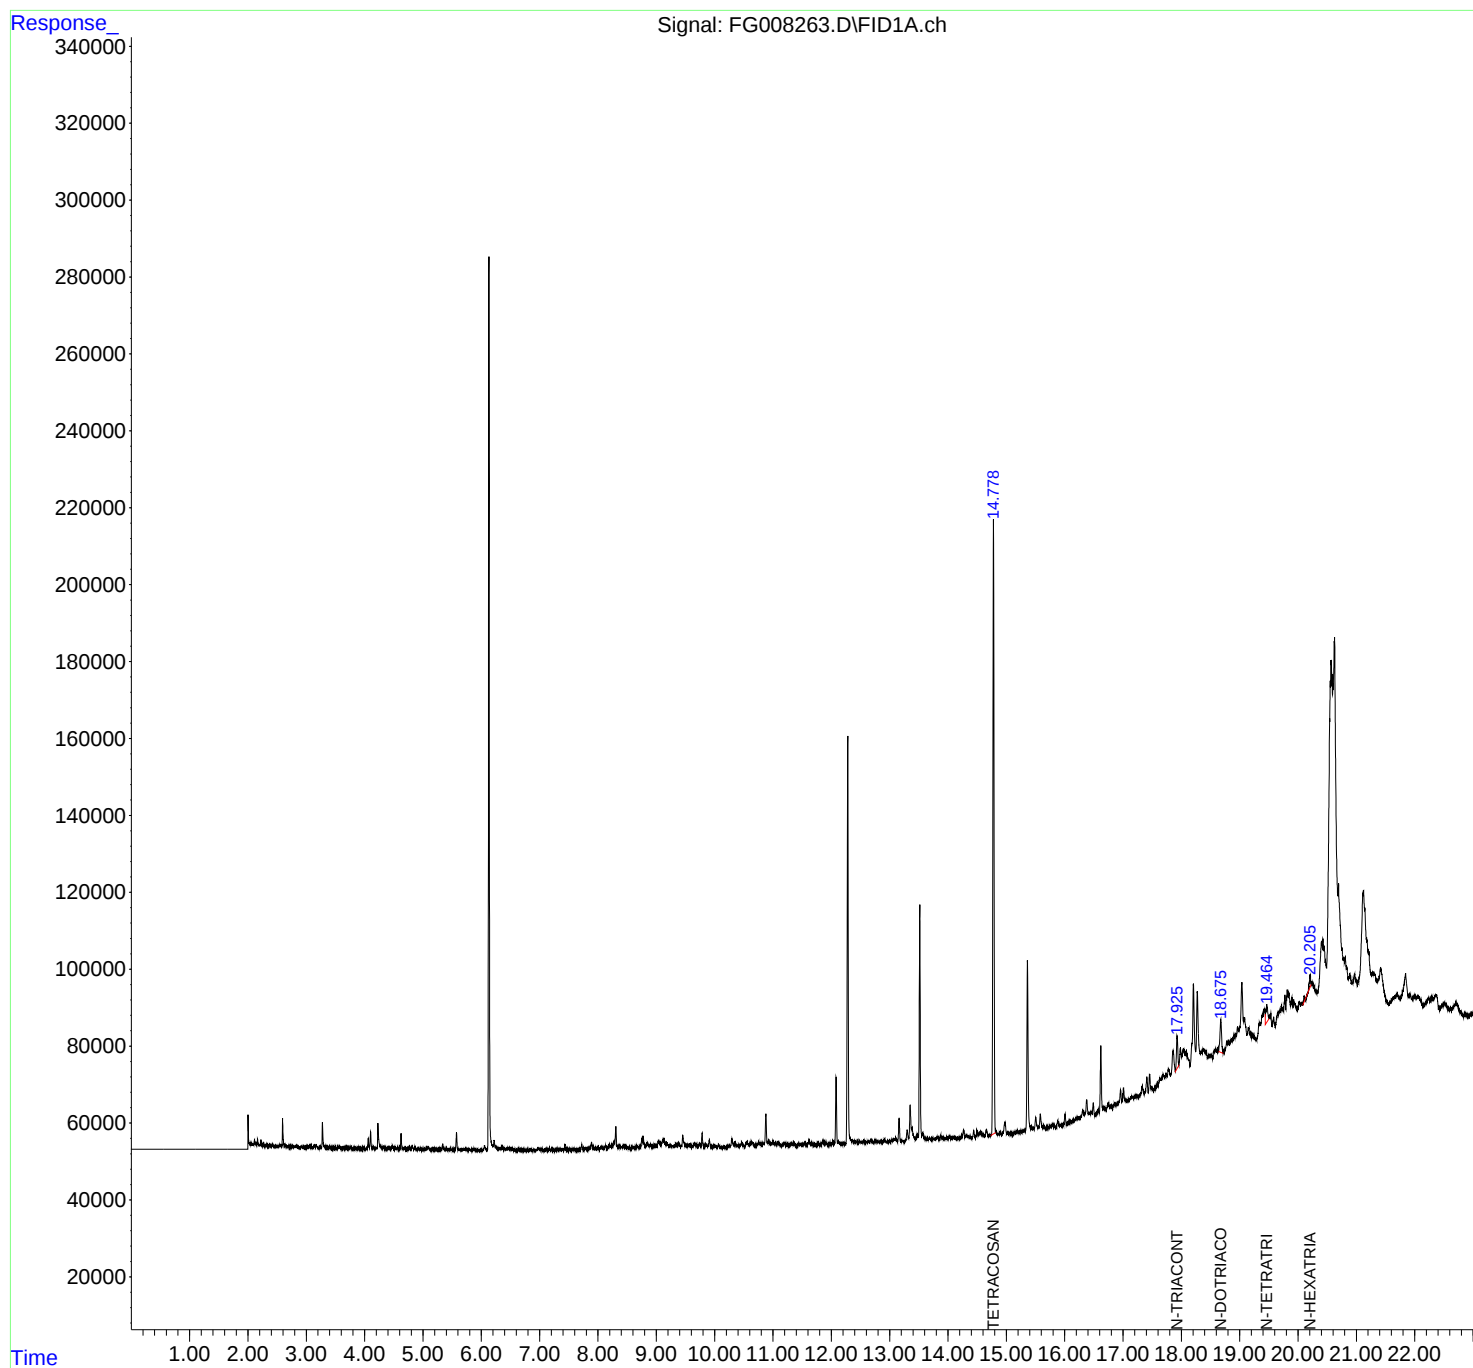


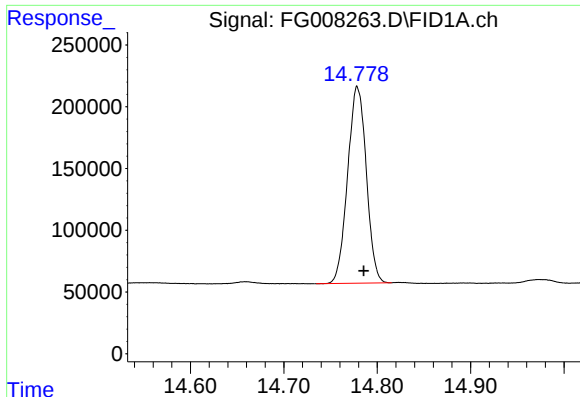

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.779 min  
Delta R.T.: -0.007 min  
Response: 2212009  
Conc: 18.64 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

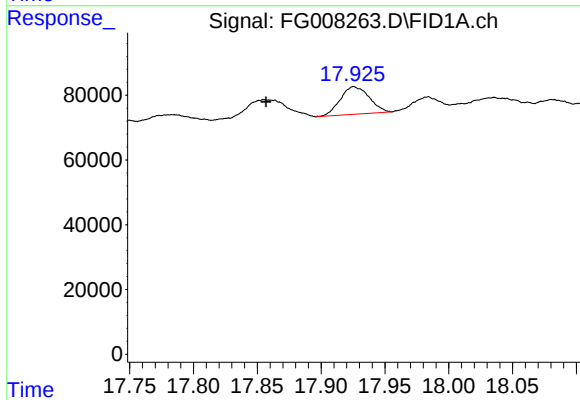


#13 N-TRIACONTANE

R.T.: 17.926 min  
Delta R.T.: 0.069 min  
Response: 133603  
Conc: 1.05 ug/ml

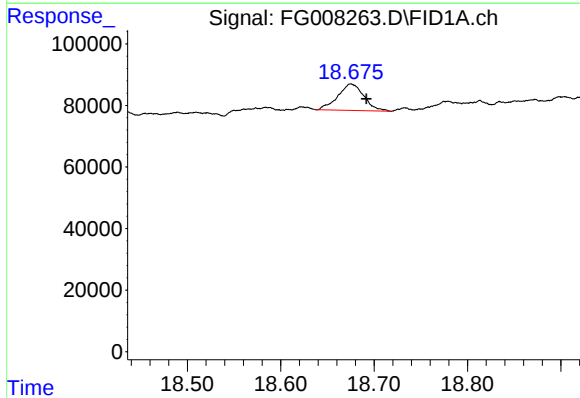


#14 N-DOTRIACONTANE

R.T.: 18.675 min  
Delta R.T.: -0.017 min  
Response: 166998  
Conc: 1.34 ug/ml

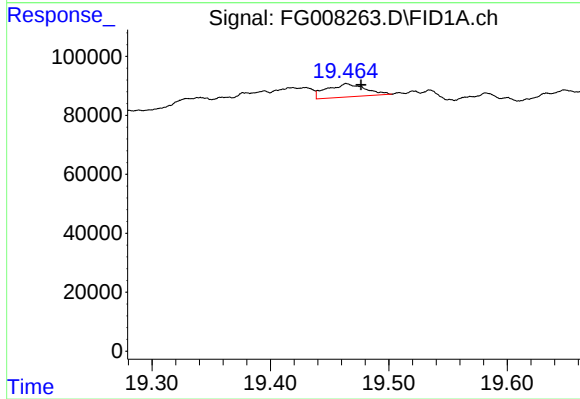

#15 N-TETRATRIACONTANE

R.T.: 19.464 min  
Delta R.T.: -0.012 min  
Response: 100578  
Conc: 0.86 ug/ml

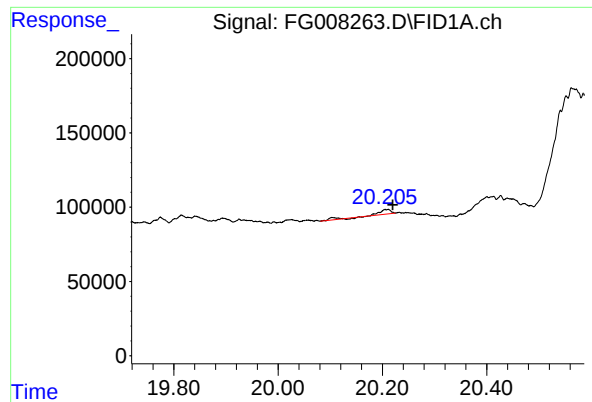

#16 N-HEXATRIACONTANE

R.T.: 20.211 min  
Delta R.T.: -0.009 min  
Response: 57378  
Conc: 0.52 ug/ml

Instrument :  
FID\_G  
ClientSampleId :