

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060921\
Data File : FG008264.D
Signal(s) : FID1A.ch
Acq On : 09 Jun 2021 20:41
Operator : DD\AJ
Sample : M2625-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 10 01:59:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.778	2360093	19.887 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.678	140088	1.127 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060921\
Data File : FG008264.D
Signal(s) : FID1A.ch
Acq On : 09 Jun 2021 20:41
Operator : DD\AJ
Sample : M2625-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 10 01:59:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

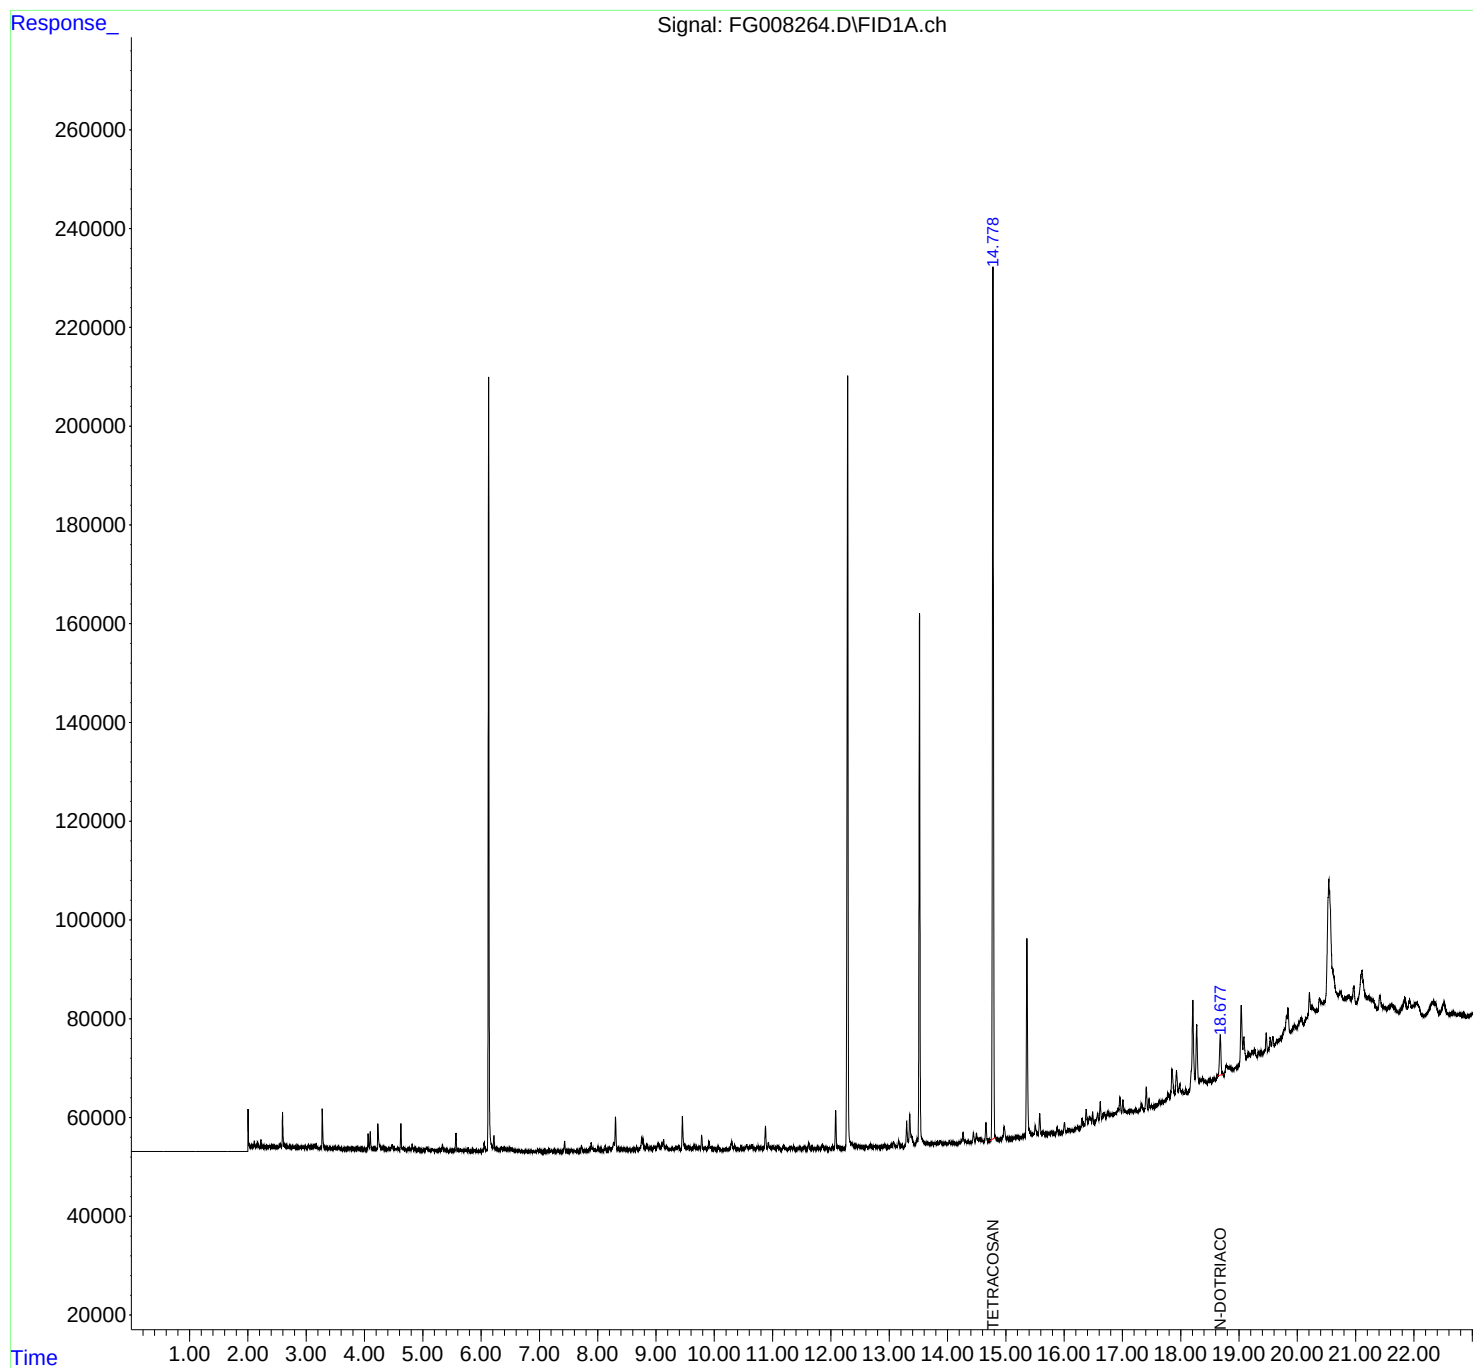


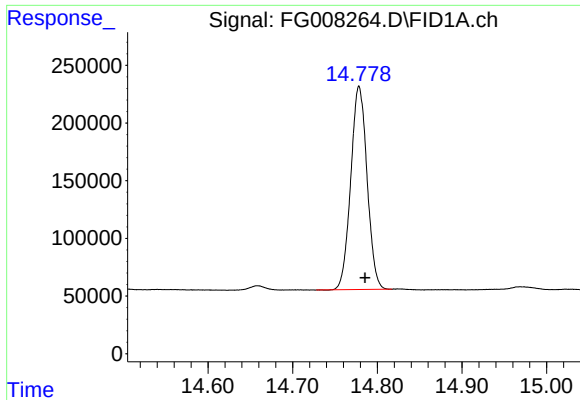

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.778 min
Delta R.T.: -0.007 min
Response: 2360093
Conc: 19.89 ug/ml

Instrument :
FID_G
ClientSampleId :

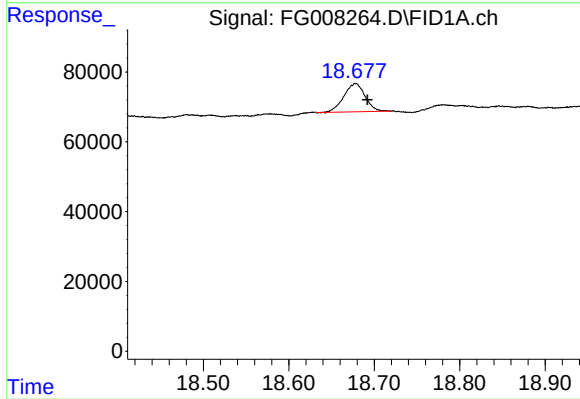

#14 N-DOTRIACONTANE

R.T.: 18.678 min
Delta R.T.: -0.013 min
Response: 140088
Conc: 1.13 ug/ml