

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060921\
Data File : FG008269.D
Signal(s) : FID1A.ch
Acq On : 09 Jun 2021 23:20
Operator : DD\AJ
Sample : M2625-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 10 02:00:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.778	2273678	19.159 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.677	153323	1.234 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060921\
Data File : FG008269.D
Signal(s) : FID1A.ch
Acq On : 09 Jun 2021 23:20
Operator : DD\AJ
Sample : M2625-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 10 02:00:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

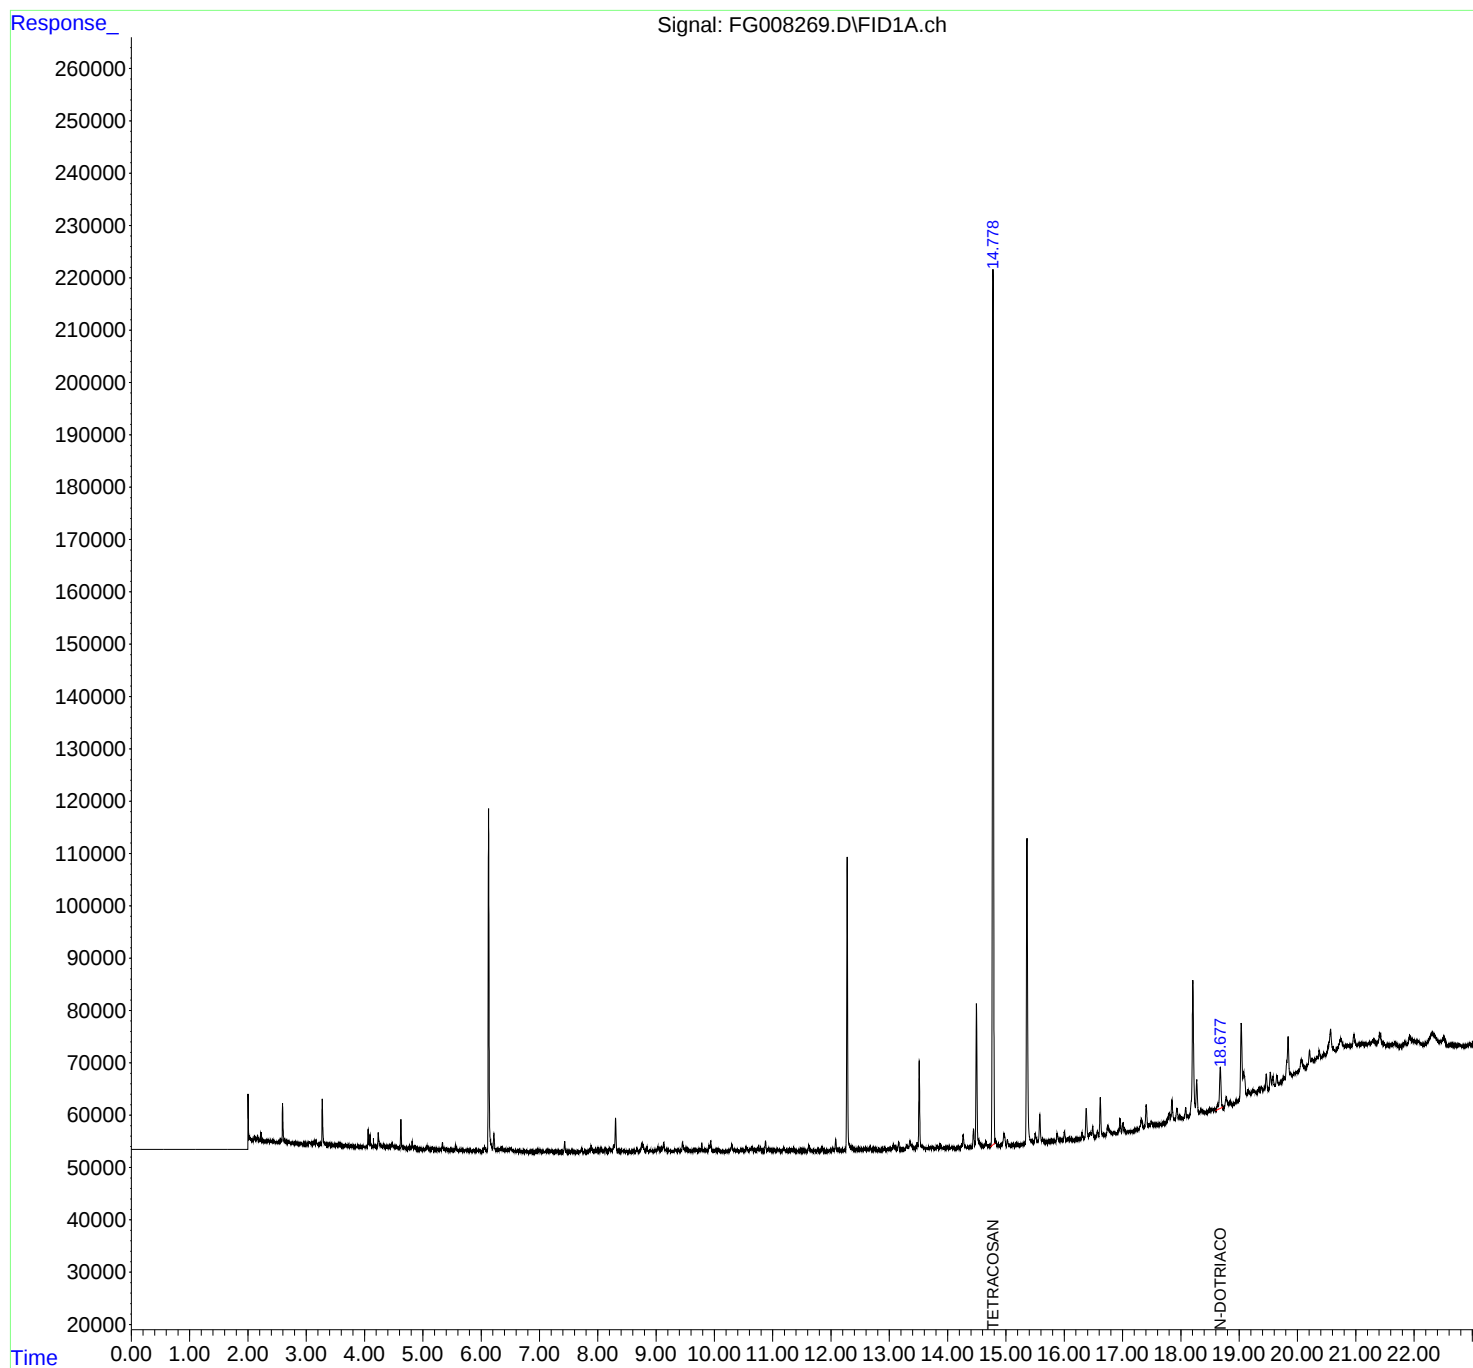


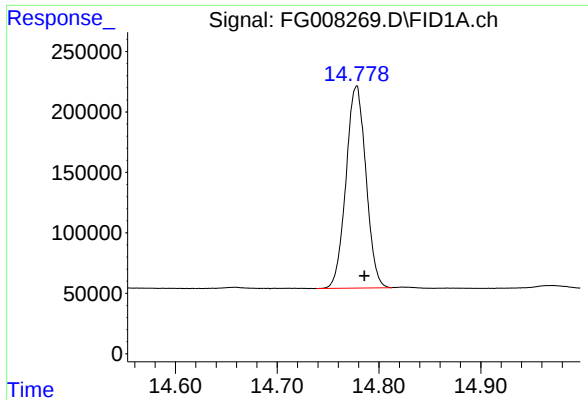

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.778 min
Delta R.T.: -0.008 min
Response: 2273678
Conc: 19.16 ug/ml

Instrument :
FID_G
ClientSampleId :

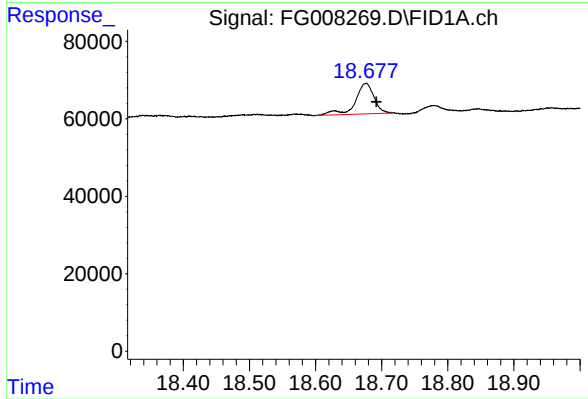

#14 N-DOTRIACONTANE

R.T.: 18.677 min
Delta R.T.: -0.015 min
Response: 153323
Conc: 1.23 ug/ml