

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060923\
 Data File : FG012137.D
 Signal(s) : FID1A.ch
 Acq On : 09 Jun 2023 13:01
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Jun 09 23:45:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
 Quant Title :
 QLast Update : Thu Jun 01 17:30:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.014	5812576	43.595 ug/ml
Target Compounds			
2) N-DECANE	4.545	7068565	47.974 ug/ml
3) N-DODECANE	6.716	7210334	48.036 ug/ml
4) N-TETRADECANE	8.545	7222788	48.209 ug/ml
5) N-HEXADECANE	10.156	7388800	47.224 ug/ml
6) N-OCTADECANE	11.601	7371605	46.353 ug/ml
7) N-EICOSANE	12.914	7224654	45.527 ug/ml
8) N-DOCOSANE	14.114	6811023	44.578 ug/ml
10) N-TETRACOSANE	15.219	6616912	44.297 ug/ml
11) N-HEXACOSANE	16.242	6369780	44.979 ug/ml
12) N-OCTACOSANE	17.194	6286741	46.440 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060923\
Data File : FG012137.D
Signal(s) : FID1A.ch
Acq On : 09 Jun 2023 13:01
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Jun 09 23:45:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

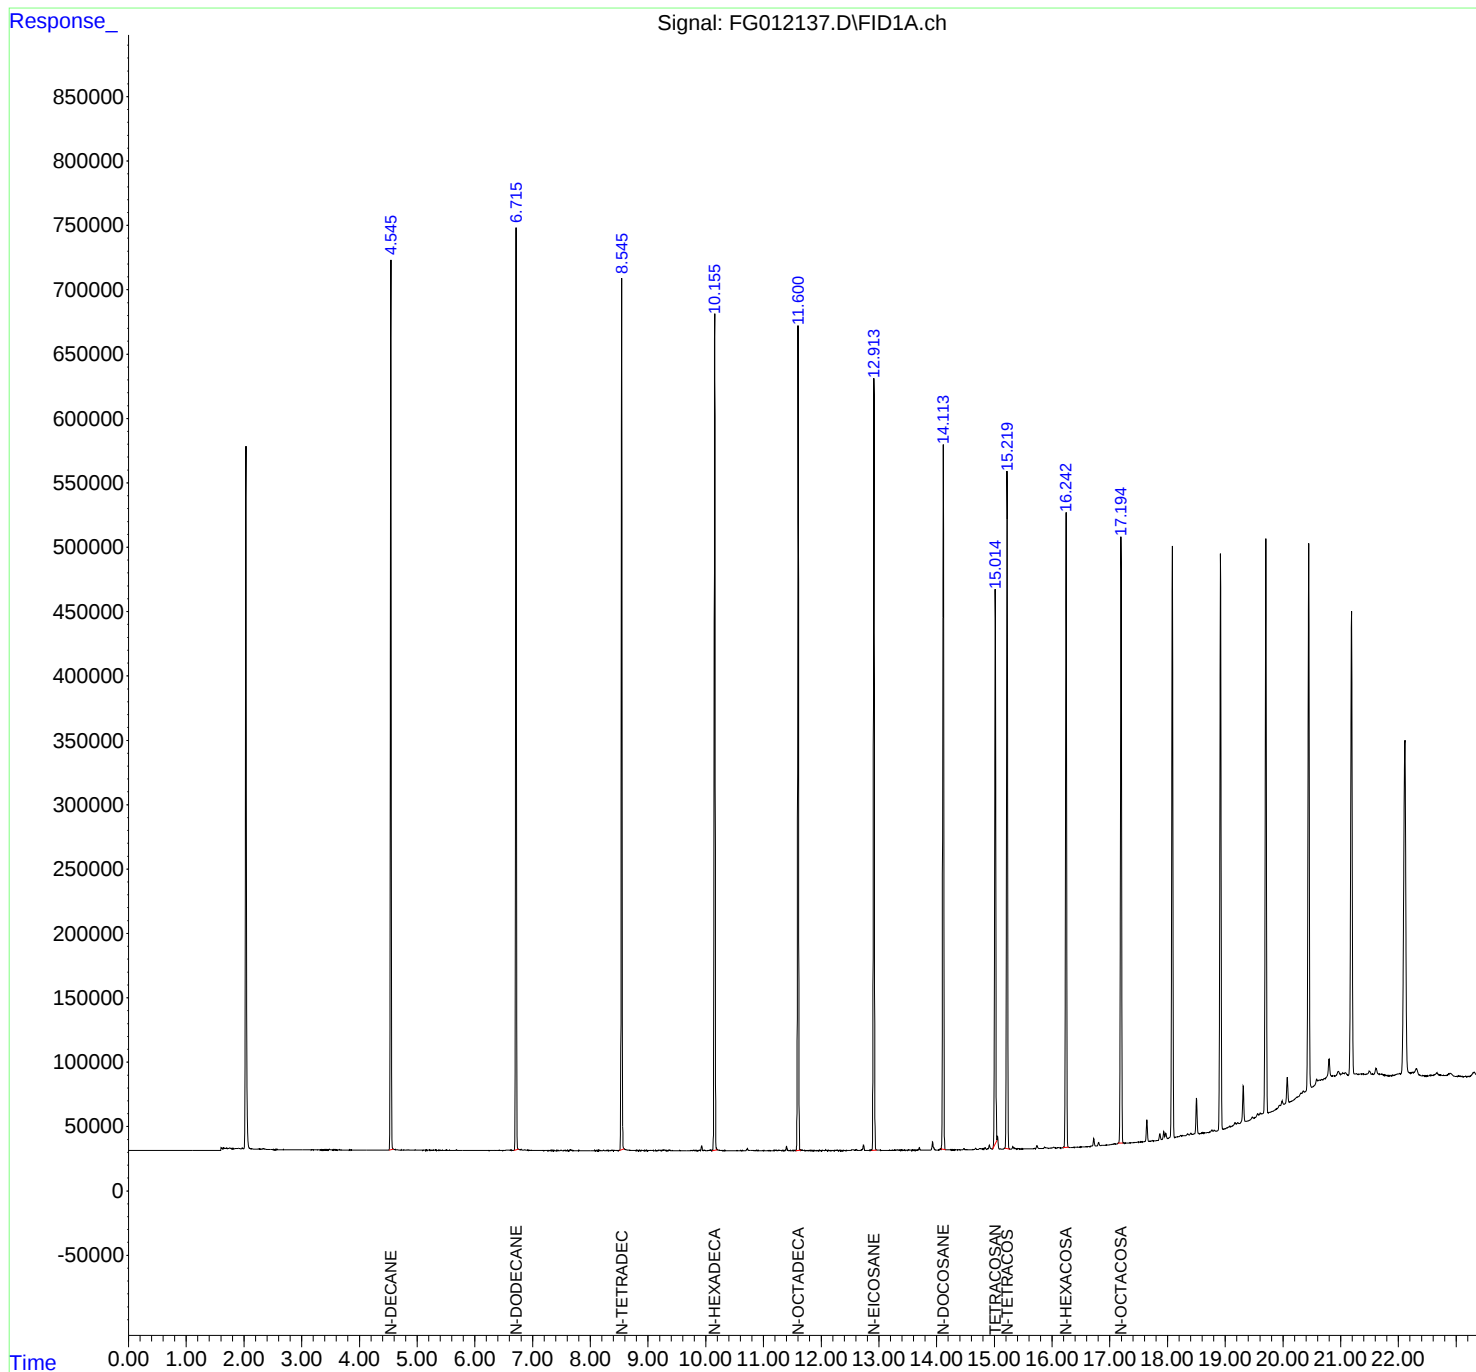


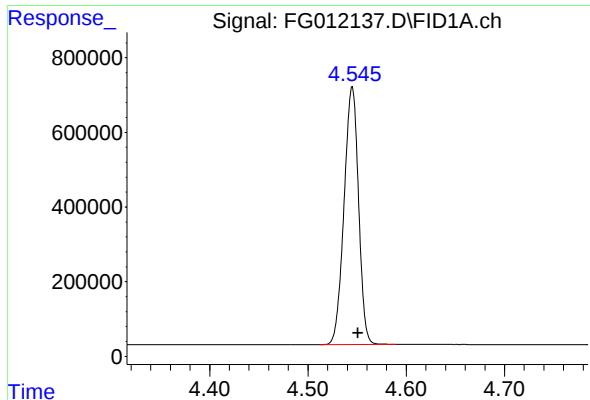

#2 N-DECANE


R.T.: 4.545 min
Delta R.T.: -0.006 min
Response: 7068565
Conc: 47.97 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

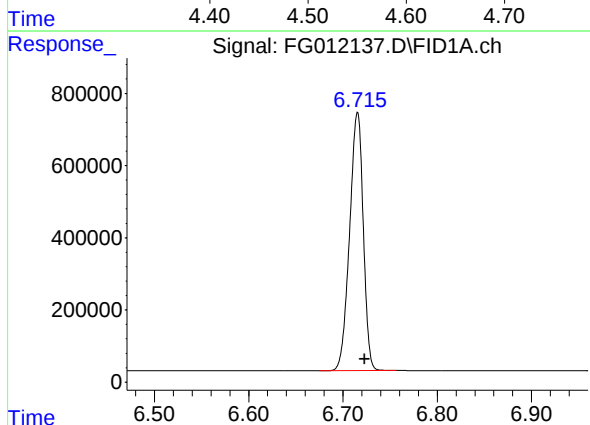


#3 N-DODECANE

R.T.: 6.716 min
Delta R.T.: -0.007 min
Response: 7210334
Conc: 48.04 ug/ml

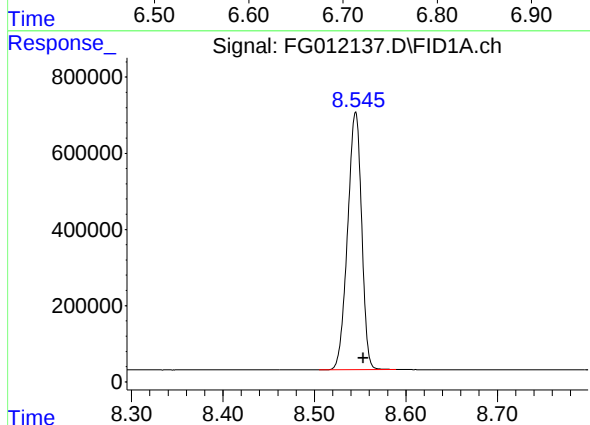


#4 N-TETRADECANE

R.T.: 8.545 min
Delta R.T.: -0.008 min
Response: 7222788
Conc: 48.21 ug/ml

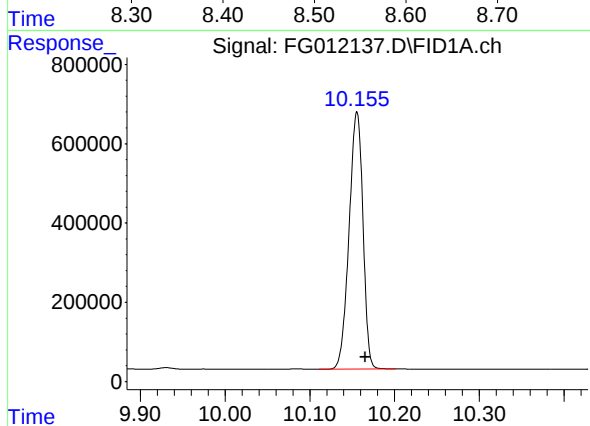

#5 N-HEXADECANE


R.T.: 10.156 min
Delta R.T.: -0.010 min
Response: 7388800
Conc: 47.22 ug/ml

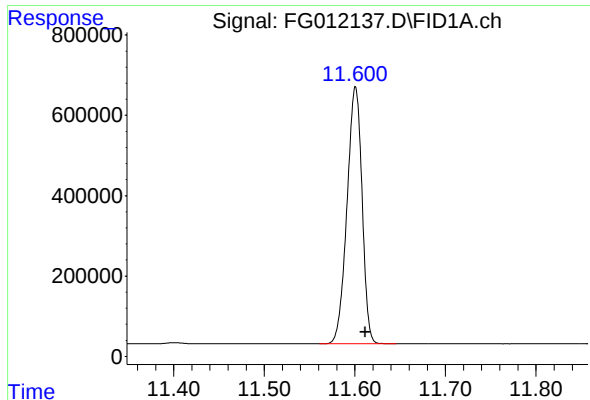

#6 N-OCTADECANE


R.T.: 11.601 min
Delta R.T.: -0.011 min
Response: 7371605
Conc: 46.35 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

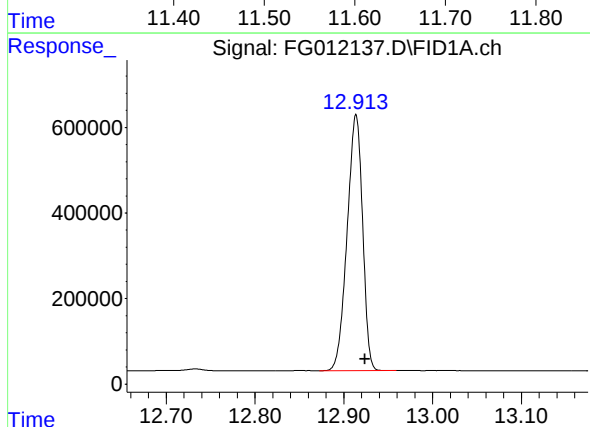


#7 N-EICOSANE

R.T.: 12.914 min
Delta R.T.: -0.010 min
Response: 7224654
Conc: 45.53 ug/ml

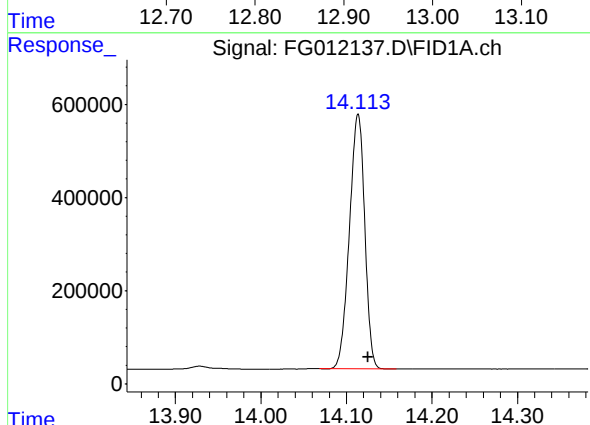


#8 N-DOCOSANE

R.T.: 14.114 min
Delta R.T.: -0.012 min
Response: 6811023
Conc: 44.58 ug/ml

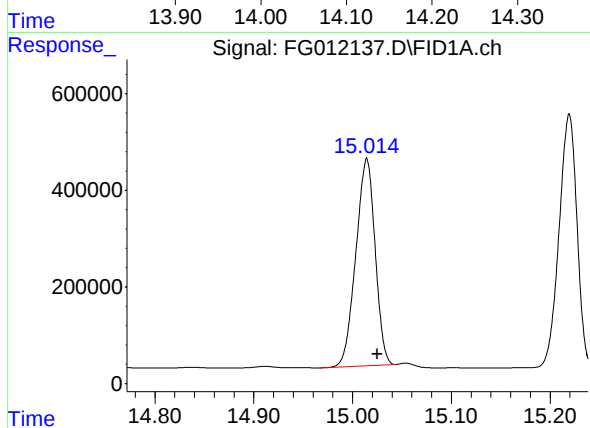

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.014 min
Delta R.T.: -0.011 min
Response: 5812576
Conc: 43.59 ug/ml

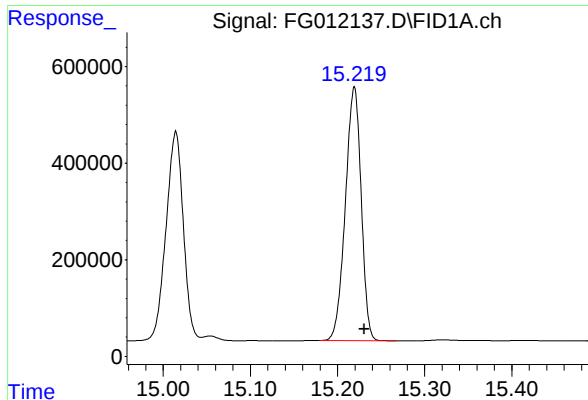

#10 N-TETRACOSANE


R.T.: 15.219 min
Delta R.T.: -0.011 min
Response: 6616912
Conc: 44.30 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

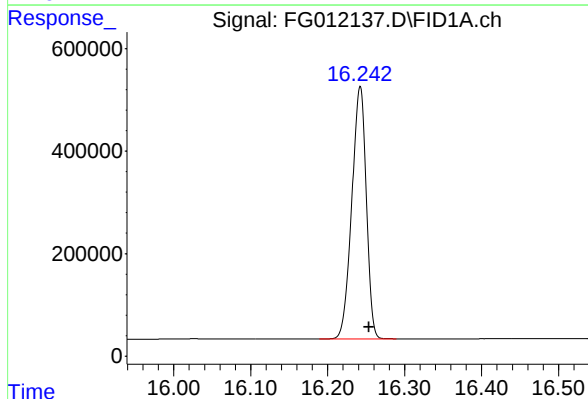

#11 N-HEXACOSANE

R.T.: 16.242 min
Delta R.T.: -0.012 min
Response: 6369780
Conc: 44.98 ug/ml

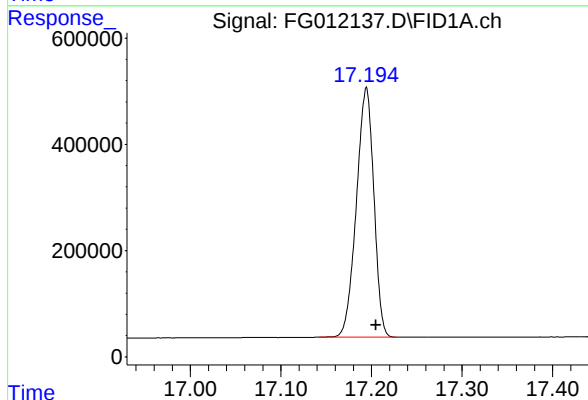

#12 N-OCTACOSANE

R.T.: 17.194 min
Delta R.T.: -0.011 min
Response: 6286741
Conc: 46.44 ug/ml