

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061025\  
Data File : FG016023.D  
Signal(s) : FID1A.ch  
Acq On : 10 Jun 2025 21:59  
Operator : YP\AJ  
Sample : PB168383BL  
Misc :  
ALS Vial : 71 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
PB168383BL

Integration File: autoint1.e  
Quant Time: Jun 11 05:55:45 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052225.M  
Quant Title :  
QLast Update : Thu May 22 06:20:25 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                          | R.T.   | Response | Conc Units   |
|-----------------------------|--------------------------|--------|----------|--------------|
| -----                       |                          |        |          |              |
| System Monitoring Compounds |                          |        |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.973 | 1826683  | 14.904 ug/ml |
| Target Compounds            |                          |        |          |              |
| 13)                         | N-TRIACONTANE            | 18.045 | 23716    | 0.174 ug/ml  |
| 14)                         | N-DOTRIACONTANE          | 18.880 | 32834    | 0.245 ug/ml  |
| 15)                         | N-TETRATRIACONTANE       | 19.664 | 38600    | 0.318 ug/ml  |
| 16)                         | N-HEXATRIACONTANE        | 20.411 | 37520    | 0.351 ug/ml  |
| -----                       |                          |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061025\  
Data File : FG016023.D  
Signal(s) : FID1A.ch  
Acq On : 10 Jun 2025 21:59  
Operator : YP\AJ  
Sample : PB168383BL  
Misc :  
ALS Vial : 71 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
PB168383BL

Integration File: autoint1.e  
Quant Time: Jun 11 05:55:45 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052225.M  
Quant Title :  
QLast Update : Thu May 22 06:20:25 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

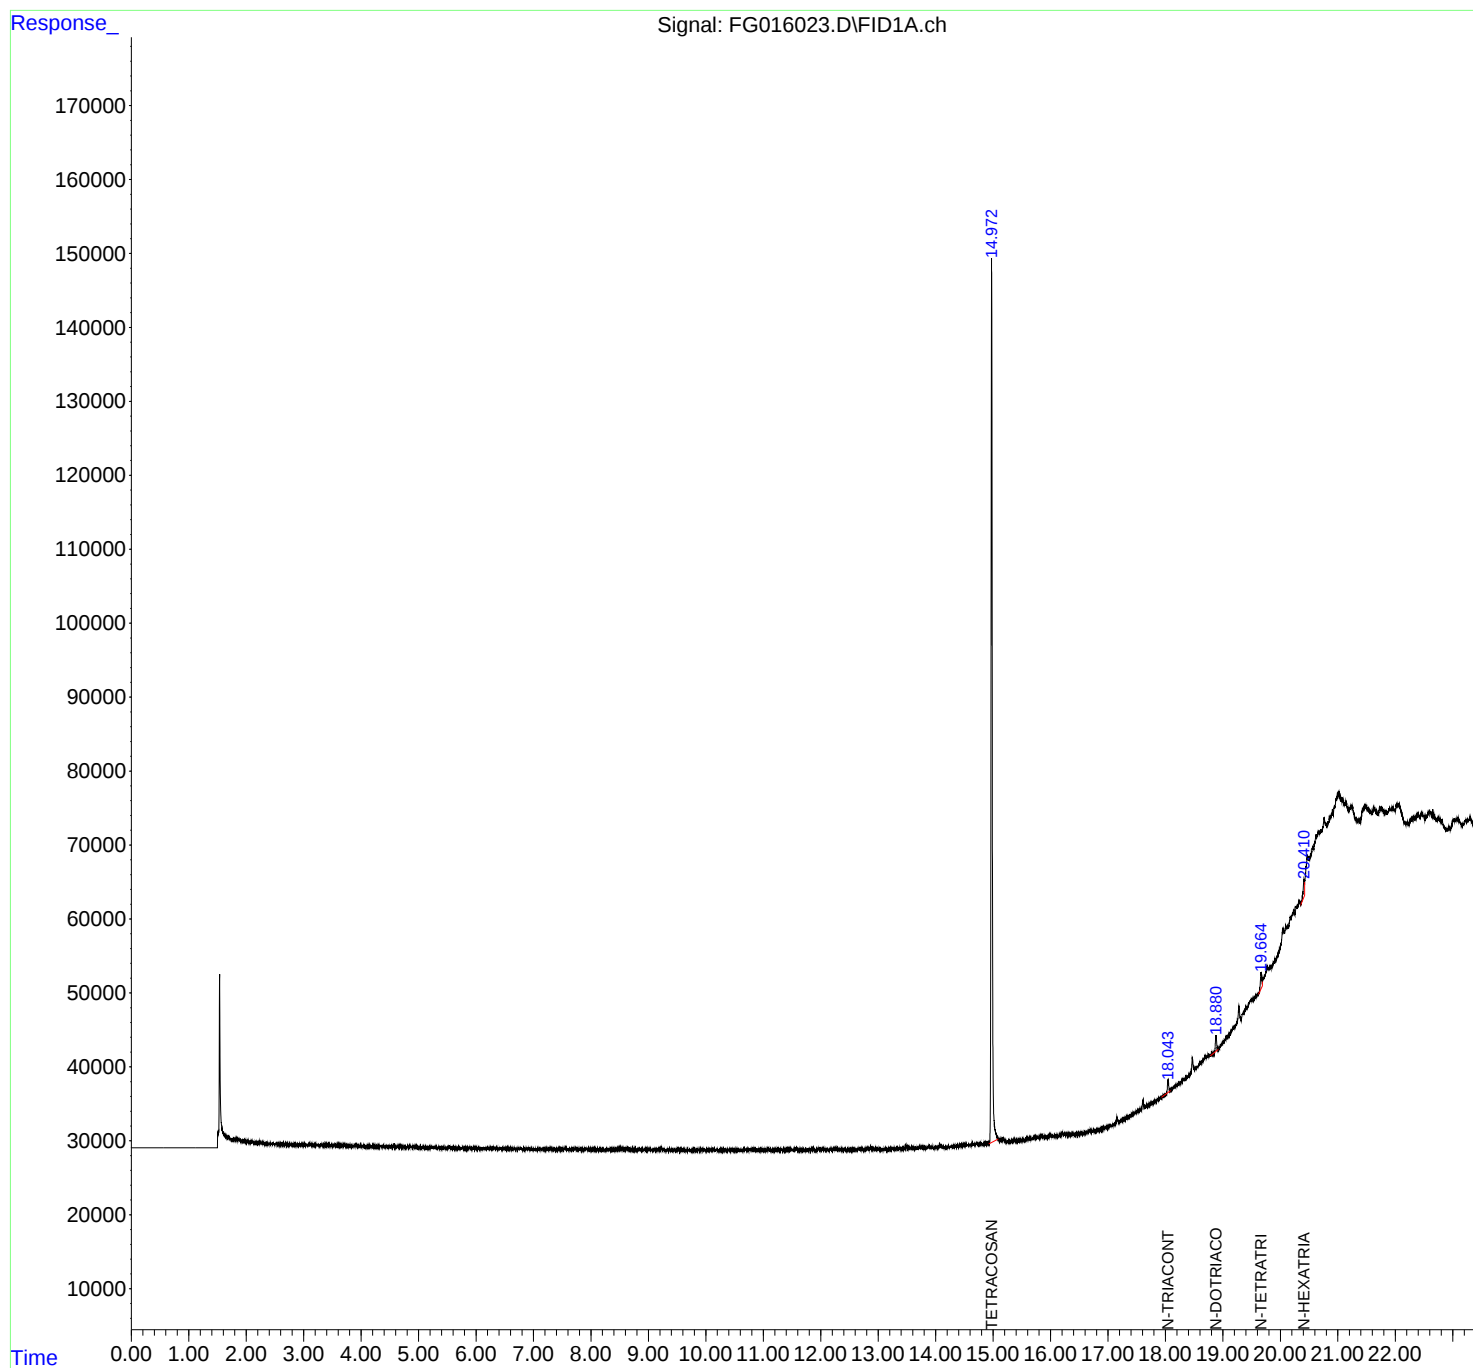


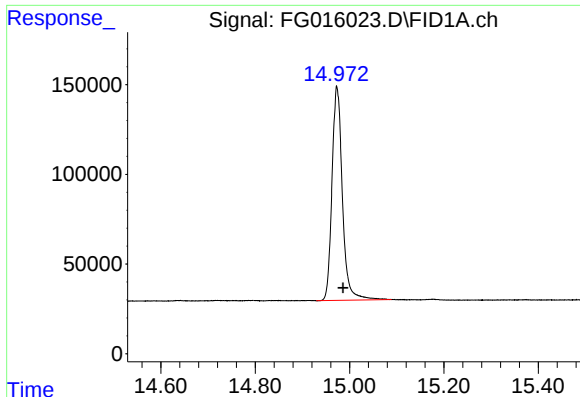

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.973 min  
Delta R.T.: -0.013 min  
Response: 1826683  
Conc: 14.90 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
PB168383BL

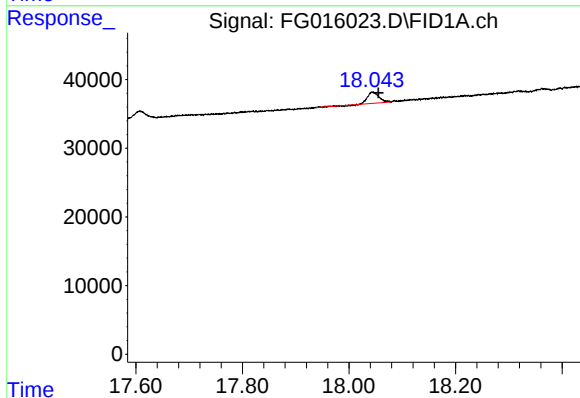


#13 N-TRIACONTANE

R.T.: 18.045 min  
Delta R.T.: -0.011 min  
Response: 23716  
Conc: 0.17 ug/ml

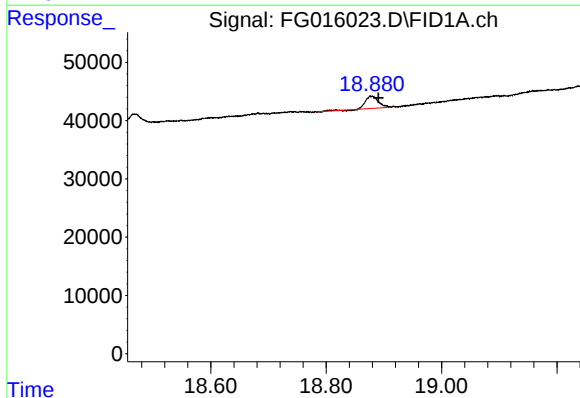


#14 N-DOTRIACONTANE

R.T.: 18.880 min  
Delta R.T.: -0.011 min  
Response: 32834  
Conc: 0.25 ug/ml

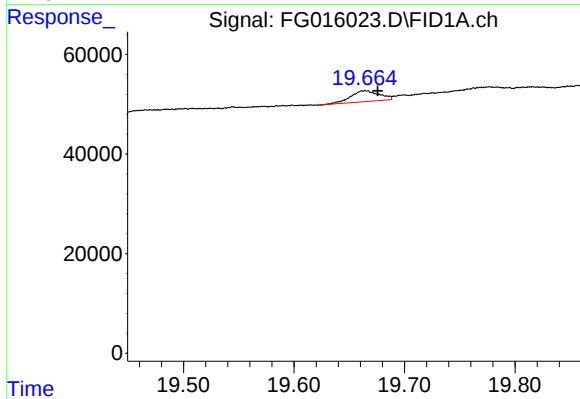

#15 N-TETRATRIACONTANE

R.T.: 19.664 min  
Delta R.T.: -0.011 min  
Response: 38600  
Conc: 0.32 ug/ml

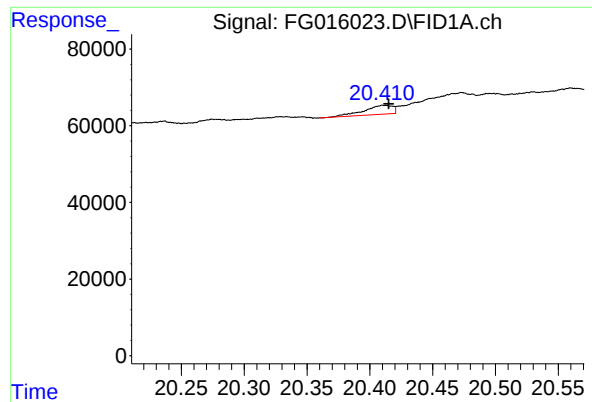

#16 N-HEXATRIACONTANE

R.T.: 20.411 min  
Delta R.T.: -0.004 min  
Response: 37520  
Conc: 0.35 ug/ml

Instrument :

FID\_G

ClientSampleId :

PB168383BL