

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061025\
 Data File : FG016024.D
 Signal(s) : FID1A.ch
 Acq On : 10 Jun 2025 22:28
 Operator : YP\AJ
 Sample : Q2126-10
 Misc : 1 PPM WATER LOD
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 LOD-MDL-WATER-04-QT2-2025

Integration File: autoint1.e
 Quant Time: Jun 11 05:56:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052225.M
 Quant Title :
 QLast Update : Thu May 22 06:20:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.971	2130587	17.384 ug/ml
Target Compounds			
1) N-OCTANE	1.952	92399	0.786 ug/ml
2) N-DECANE	4.476	80971	0.689 ug/ml
3) N-DODECANE	6.659	64762	0.534 ug/ml
4) N-TETRADECANE	8.497	71798	0.562 ug/ml
5) N-HEXADECANE	10.112	83803	0.629 ug/ml
6) N-OCTADECANE	11.557	103406	0.749 ug/ml
7) N-EICOSANE	12.869	120610	0.854 ug/ml
8) N-DOCOSANE	14.069	134322	0.978 ug/ml
10) N-TETRACOSANE	15.176	134253	0.977 ug/ml
11) N-HEXACOSANE	16.201	126592	0.932 ug/ml
12) N-OCTACOSANE	17.153	141238	1.048 ug/ml
13) N-TRIACONTANE	18.043	168083	1.232 ug/ml
14) N-DOTRIACONTANE	18.877	180577	1.348 ug/ml
15) N-TETRATRIACONTANE	19.663	153931	1.269 ug/ml
16) N-HEXATRIACONTANE	20.403	114081	1.068 ug/ml
17) N-OCTATRIACONTANE	21.140	66458	0.693 ug/ml
18) N-TETRACONTANE	22.050	117524	1.336 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061025\
Data File : FG016024.D
Signal(s) : FID1A.ch
Acq On : 10 Jun 2025 22:28
Operator : YP\AJ
Sample : Q2126-10
Misc : 1 PPM WATER LOD
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LOD-MDL-WATER-04-QT2-2025

Integration File: autoint1.e
Quant Time: Jun 11 05:56:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052225.M
Quant Title :
QLast Update : Thu May 22 06:20:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

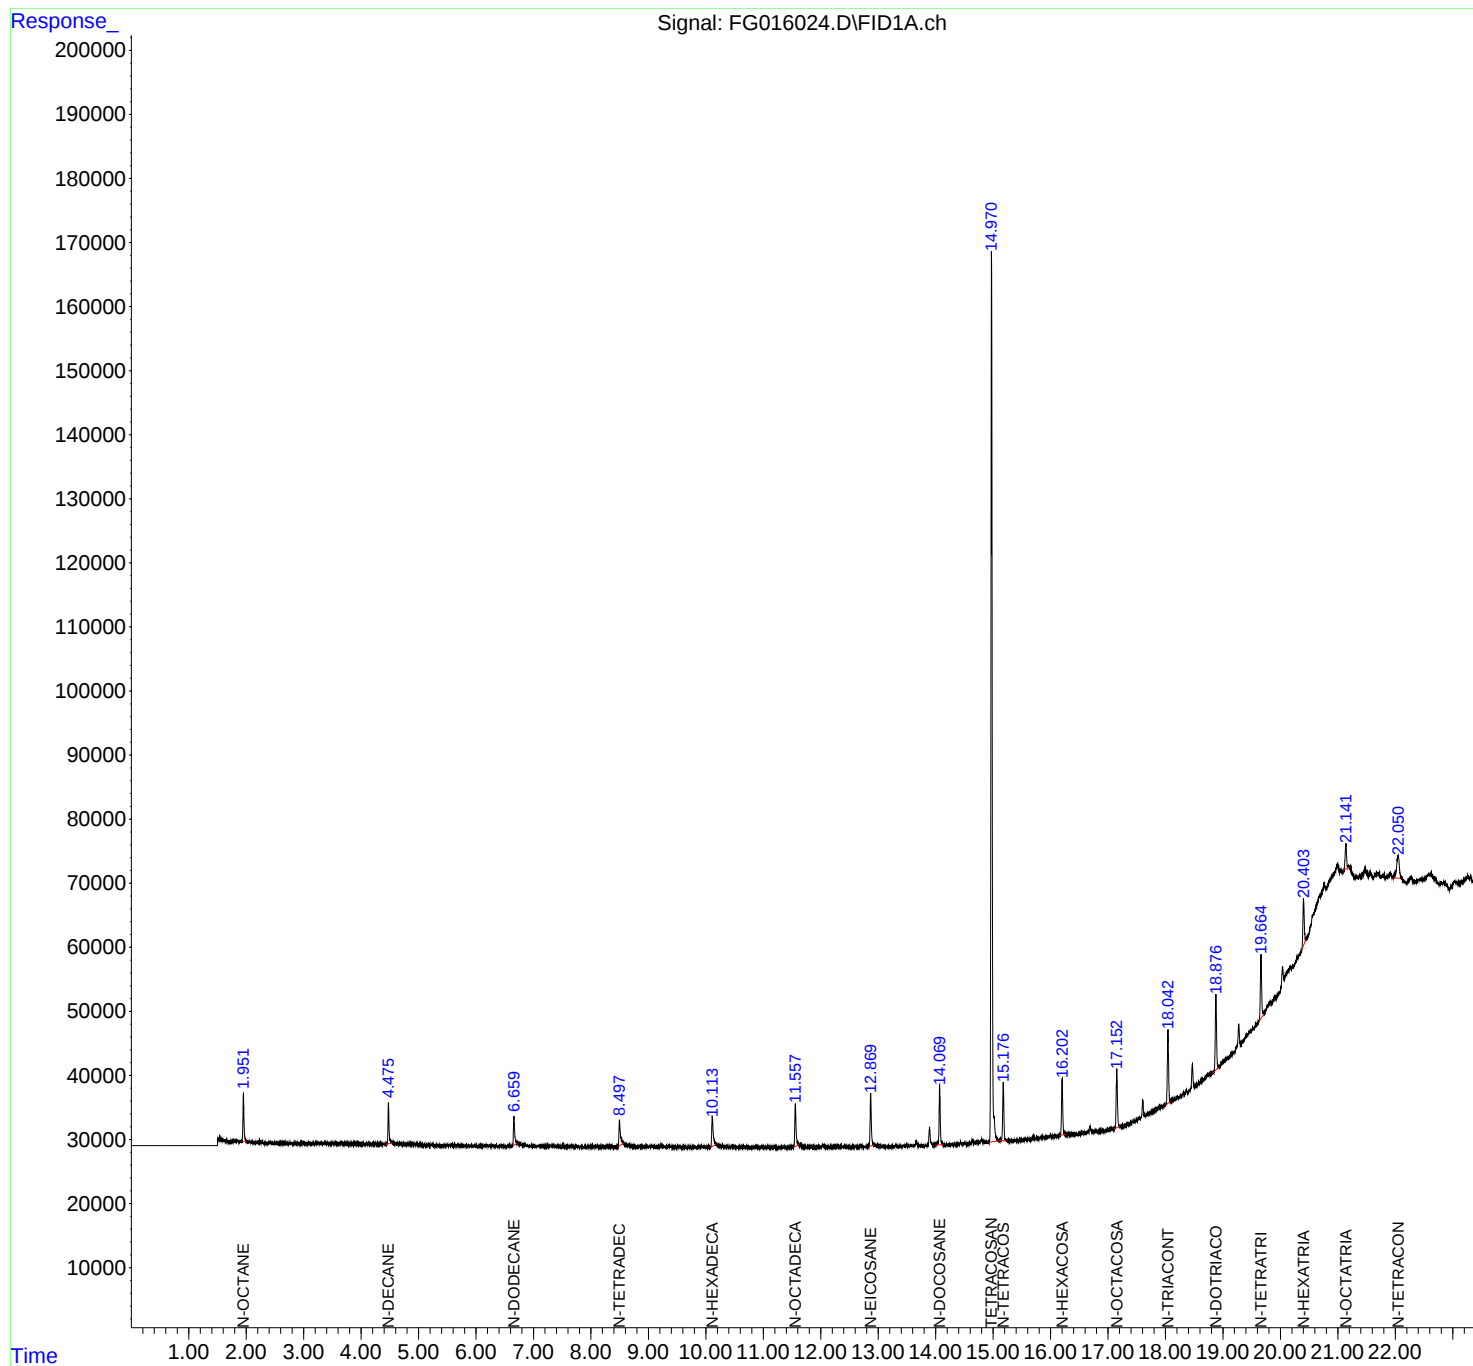


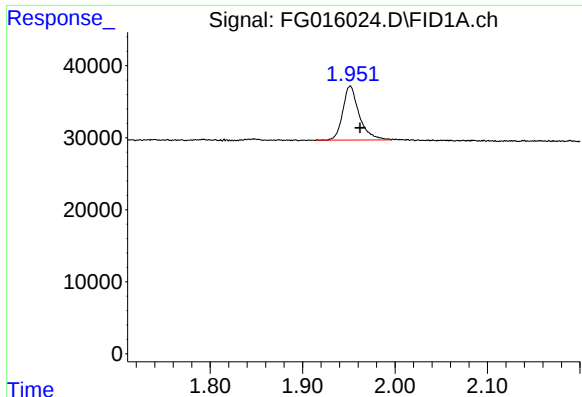

#1 N-OCTANE


R.T.: 1.952 min
Delta R.T.: -0.010 min
Response: 92399
Conc: 0.79 ug/ml

Instrument :
FID_G
ClientSampleId :
LOD-MDL-WATER-04-QT2-2025

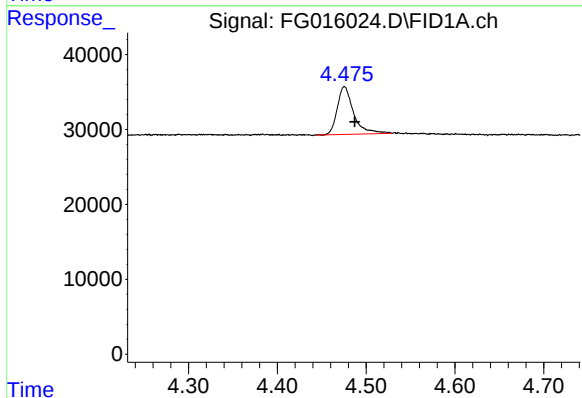


#2 N-DECANE

R.T.: 4.476 min
Delta R.T.: -0.012 min
Response: 80971
Conc: 0.69 ug/ml

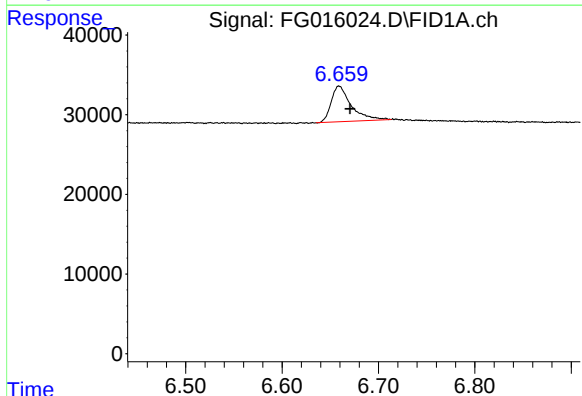


#3 N-DODECANE

R.T.: 6.659 min
Delta R.T.: -0.011 min
Response: 64762
Conc: 0.53 ug/ml

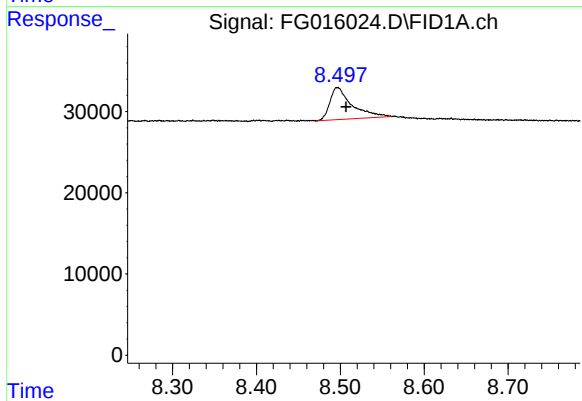

#4 N-TETRADECANE


R.T.: 8.497 min
Delta R.T.: -0.010 min
Response: 71798
Conc: 0.56 ug/ml

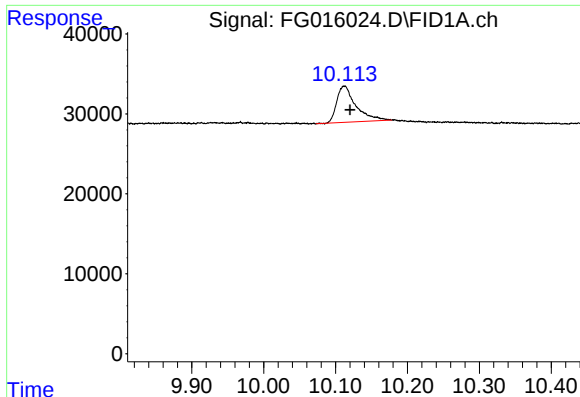

#5 N-HEXADECANE


R.T.: 10.112 min
Delta R.T.: -0.008 min
Response: 83803
Conc: 0.63 ug/ml

Instrument :
FID_G
ClientSampleId :
LOD-MDL-WATER-04-QT2-2025

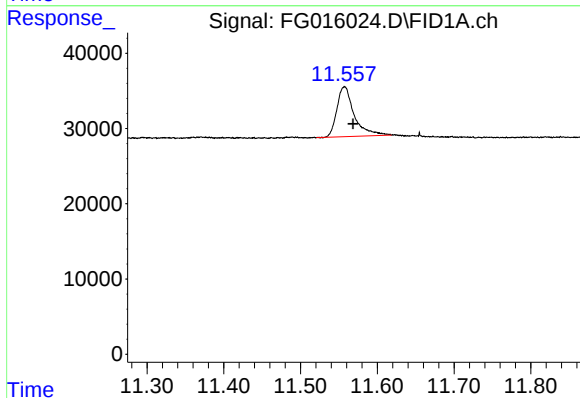


#6 N-OCTADECANE

R.T.: 11.557 min
Delta R.T.: -0.011 min
Response: 103406
Conc: 0.75 ug/ml

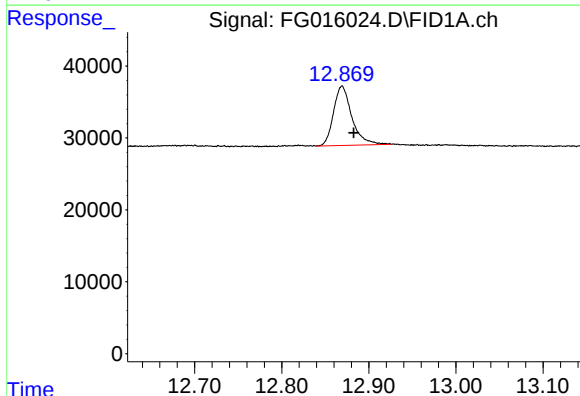


#7 N-EICOSANE

R.T.: 12.869 min
Delta R.T.: -0.013 min
Response: 120610
Conc: 0.85 ug/ml

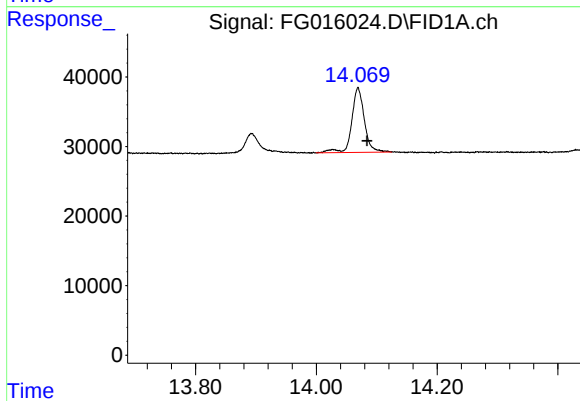

#8 N-DOCOSANE


R.T.: 14.069 min
Delta R.T.: -0.015 min
Response: 134322
Conc: 0.98 ug/ml

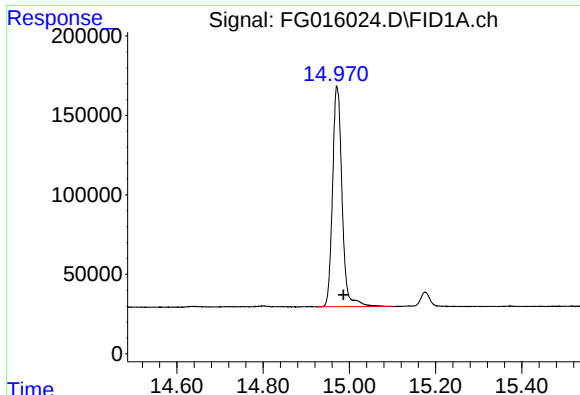

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.971 min
Delta R.T.: -0.015 min
Response: 2130587
Conc: 17.38 ug/ml

Instrument :
FID_G
ClientSampleId :
LOD-MDL-WATER-04-QT2-2025

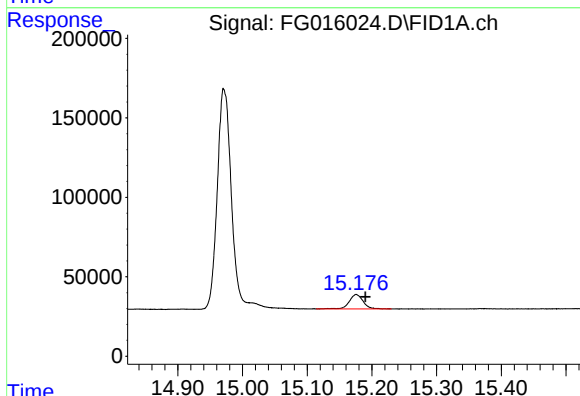


#10 N-TETRACOSANE

R.T.: 15.176 min
Delta R.T.: -0.015 min
Response: 134253
Conc: 0.98 ug/ml

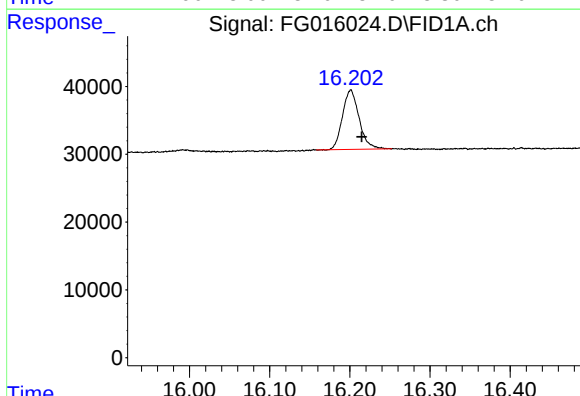


#11 N-HEXACOSANE

R.T.: 16.201 min
Delta R.T.: -0.014 min
Response: 126592
Conc: 0.93 ug/ml

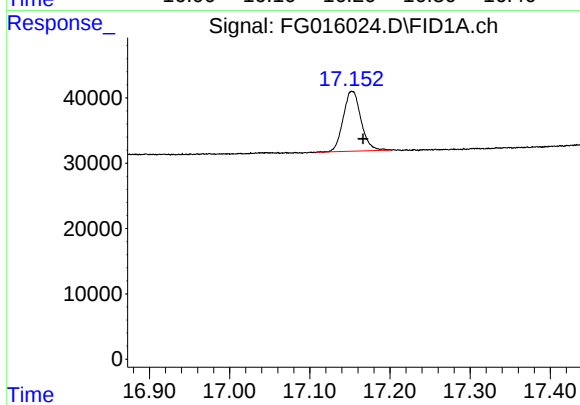

#12 N-OCTACOSANE

R.T.: 17.153 min
Delta R.T.: -0.013 min
Response: 141238
Conc: 1.05 ug/ml

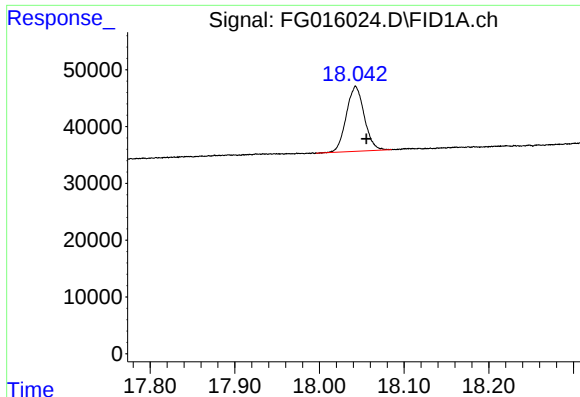

#13 N-TRIACONTANE


R.T.: 18.043 min
Delta R.T.: -0.013 min
Response: 168083
Conc: 1.23 ug/ml

Instrument :

FID_G


ClientSampleId :

LOD-MDL-WATER-04-QT2-2025

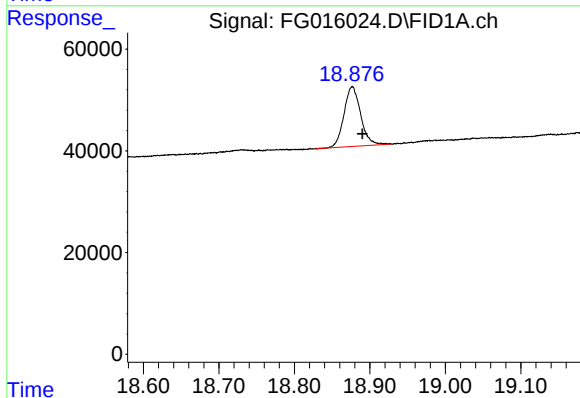


#14 N-DOTRIACONTANE

R.T.: 18.877 min
Delta R.T.: -0.014 min
Response: 180577
Conc: 1.35 ug/ml

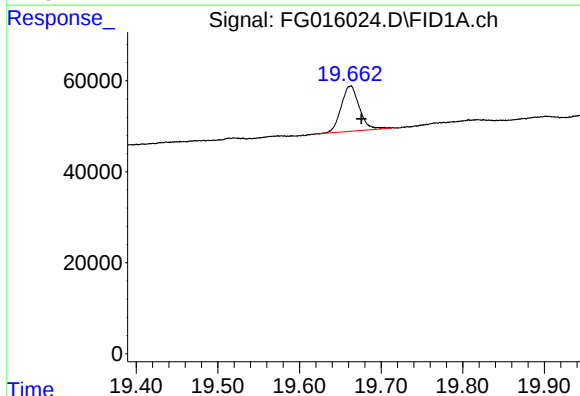


#15 N-TETRATRIACONTANE

R.T.: 19.663 min
Delta R.T.: -0.013 min
Response: 153931
Conc: 1.27 ug/ml

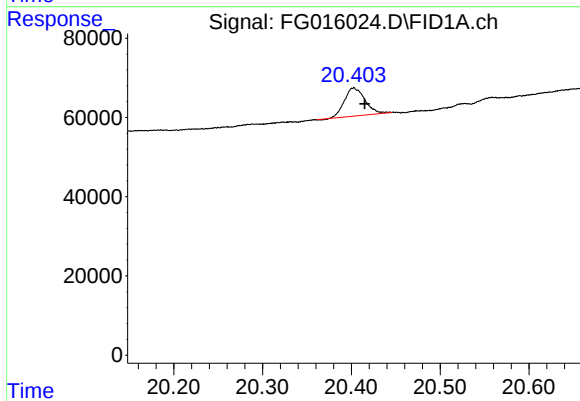

#16 N-HEXATRIACONTANE


R.T.: 20.403 min
Delta R.T.: -0.012 min
Response: 114081
Conc: 1.07 ug/ml

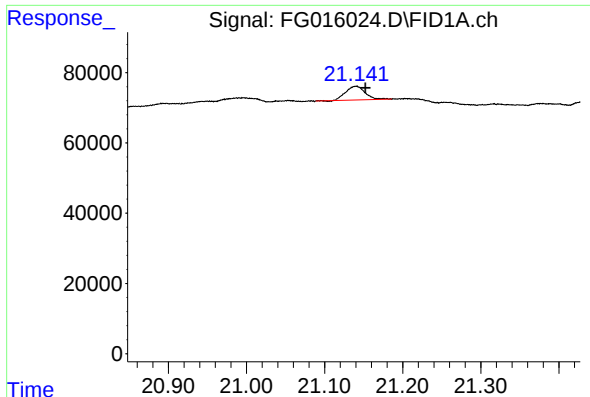

#17 N-OCTATRIACONTANE

R.T.: 21.140 min
Delta R.T.: -0.012 min
Response: 66458
Conc: 0.69 ug/ml

Instrument :
FID_G
ClientSampleId :
LOD-MDL-WATER-04-QT2-2025

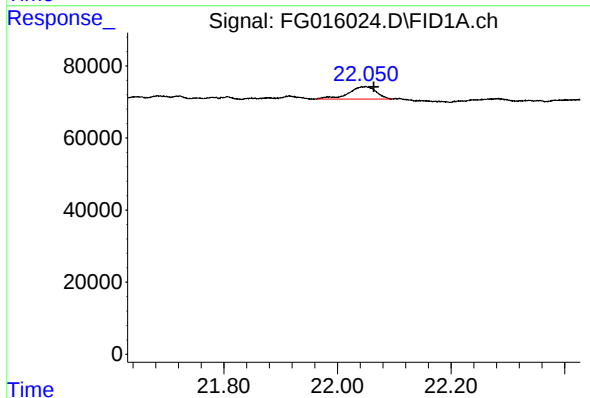

#18 N-TETRACONTANE

R.T.: 22.050 min
Delta R.T.: -0.014 min
Response: 117524
Conc: 1.34 ug/ml