

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061025\  
Data File : FG016017.D  
Signal(s) : FID1A.ch  
Acq On : 10 Jun 2025 18:32  
Operator : YP\AJ  
Sample : Q2198-03  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
B-207-SB02

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/11/2025  
Supervised By :mohammad ahmed 06/12/2025

Integration File: autoint1.e  
Quant Time: Jun 11 05:53:44 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052225.M  
Quant Title :  
QLast Update : Thu May 22 06:20:25 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.970 | 1245946  | 10.166 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061025\  
Data File : FG016017.D  
Signal(s) : FID1A.ch  
Acq On : 10 Jun 2025 18:32  
Operator : YP\AJ  
Sample : Q2198-03  
Misc :  
ALS Vial : 32 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
B-207-SB02


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/11/2025  
Supervised By :mohammad ahmed 06/12/2025

Integration File: autoint1.e  
Quant Time: Jun 11 05:53:44 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052225.M  
Quant Title :  
QLast Update : Thu May 22 06:20:25 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

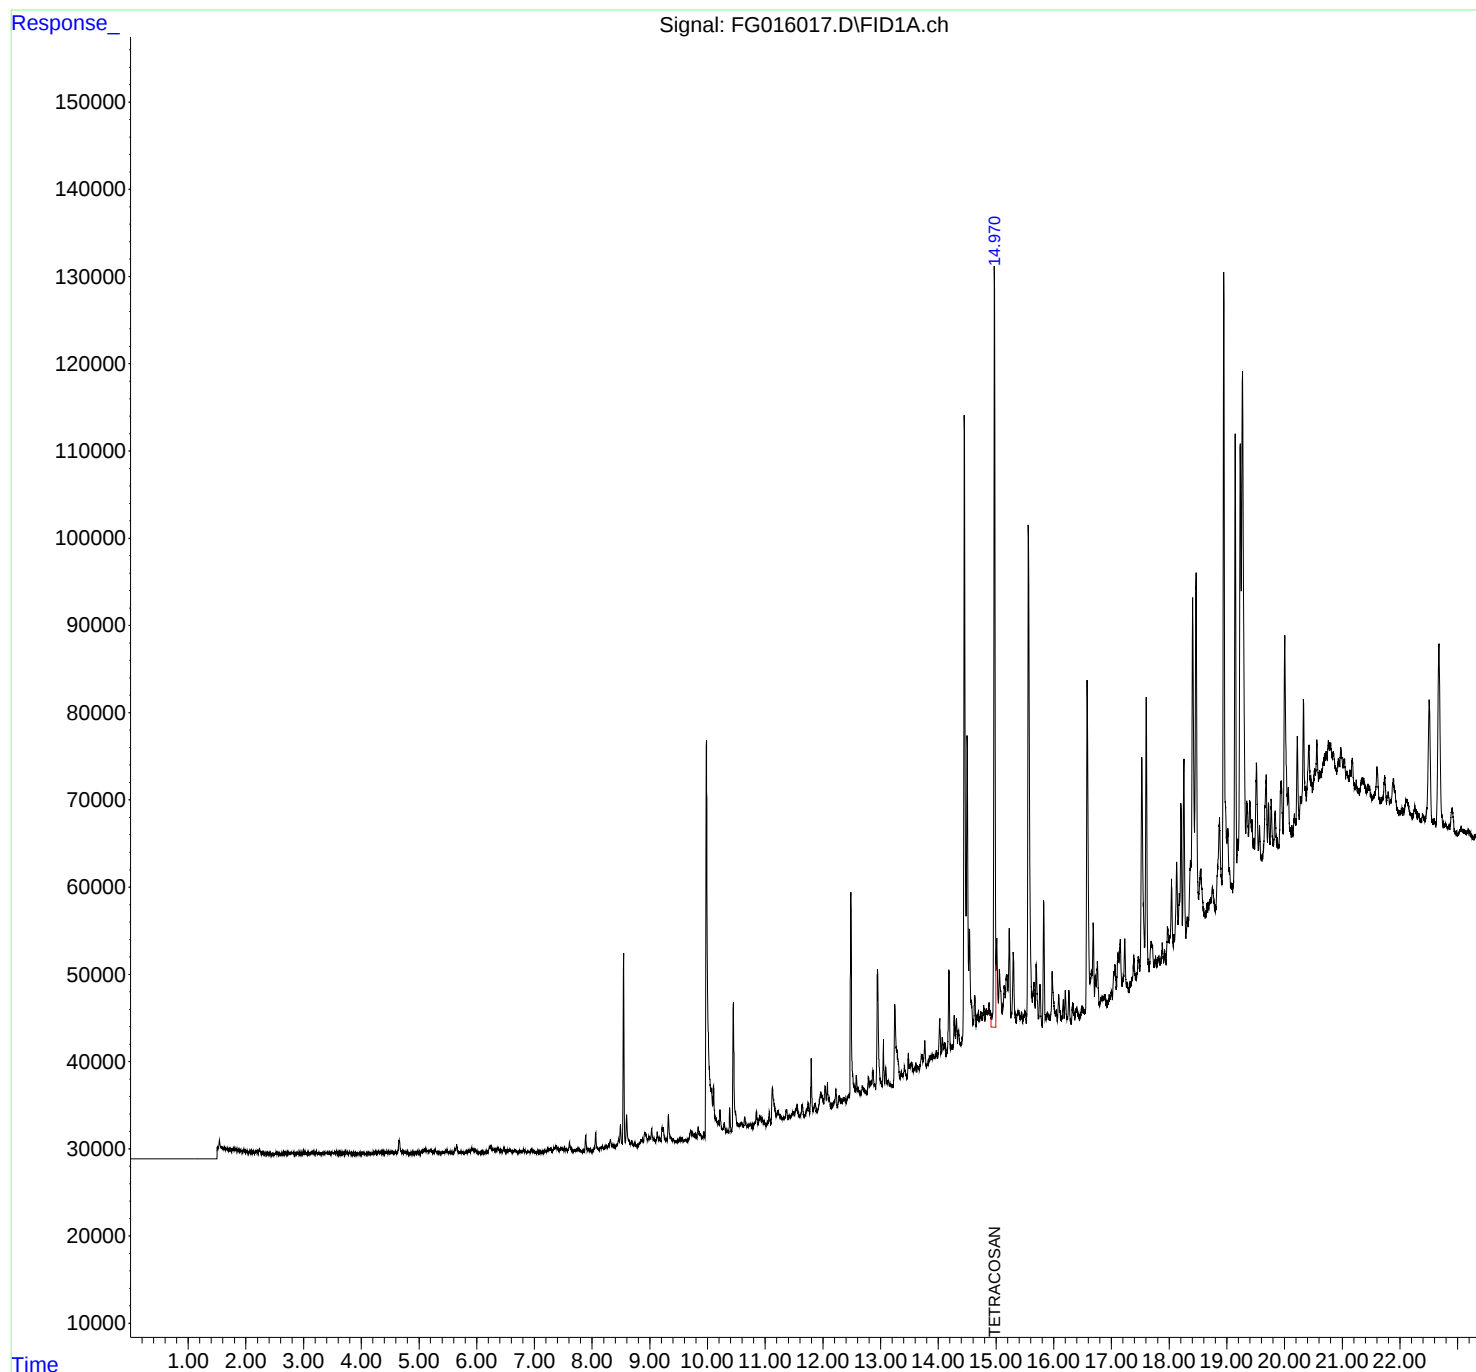

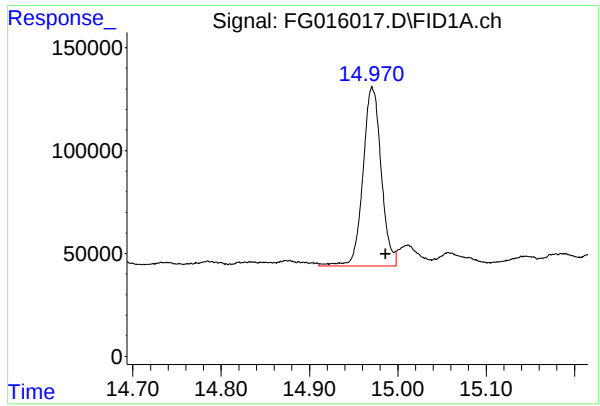

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.970 min  
Delta R.T.: -0.016 min  
Response: 1245946  
Conc: 10.17 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
B-207-SB02

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/11/2025  
Supervised By :mohammad ahmed 06/12/2025