

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061322\
 Data File : FG009864.D
 Signal(s) : FID1A.ch
 Acq On : 13 Jun 2022 17:00
 Operator : AJ\MA
 Sample : N3304-02 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 WC-14A-1A-10-G

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/14/2022
 Supervised By :Ankita Jodhani 06/14/2022

Integration File: autoint1.e
 Quant Time: Jun 14 06:37:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
 Quant Title :
 QLast Update : Wed Jun 01 13:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.837	63180	0.600 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061322\
Data File : FG009864.D
Signal(s) : FID1A.ch
Acq On : 13 Jun 2022 17:00
Operator : AJ\MA
Sample : N3304-02 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
WC-14A-1A-10-G


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

Integration File: autoint1.e
Quant Time: Jun 14 06:37:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

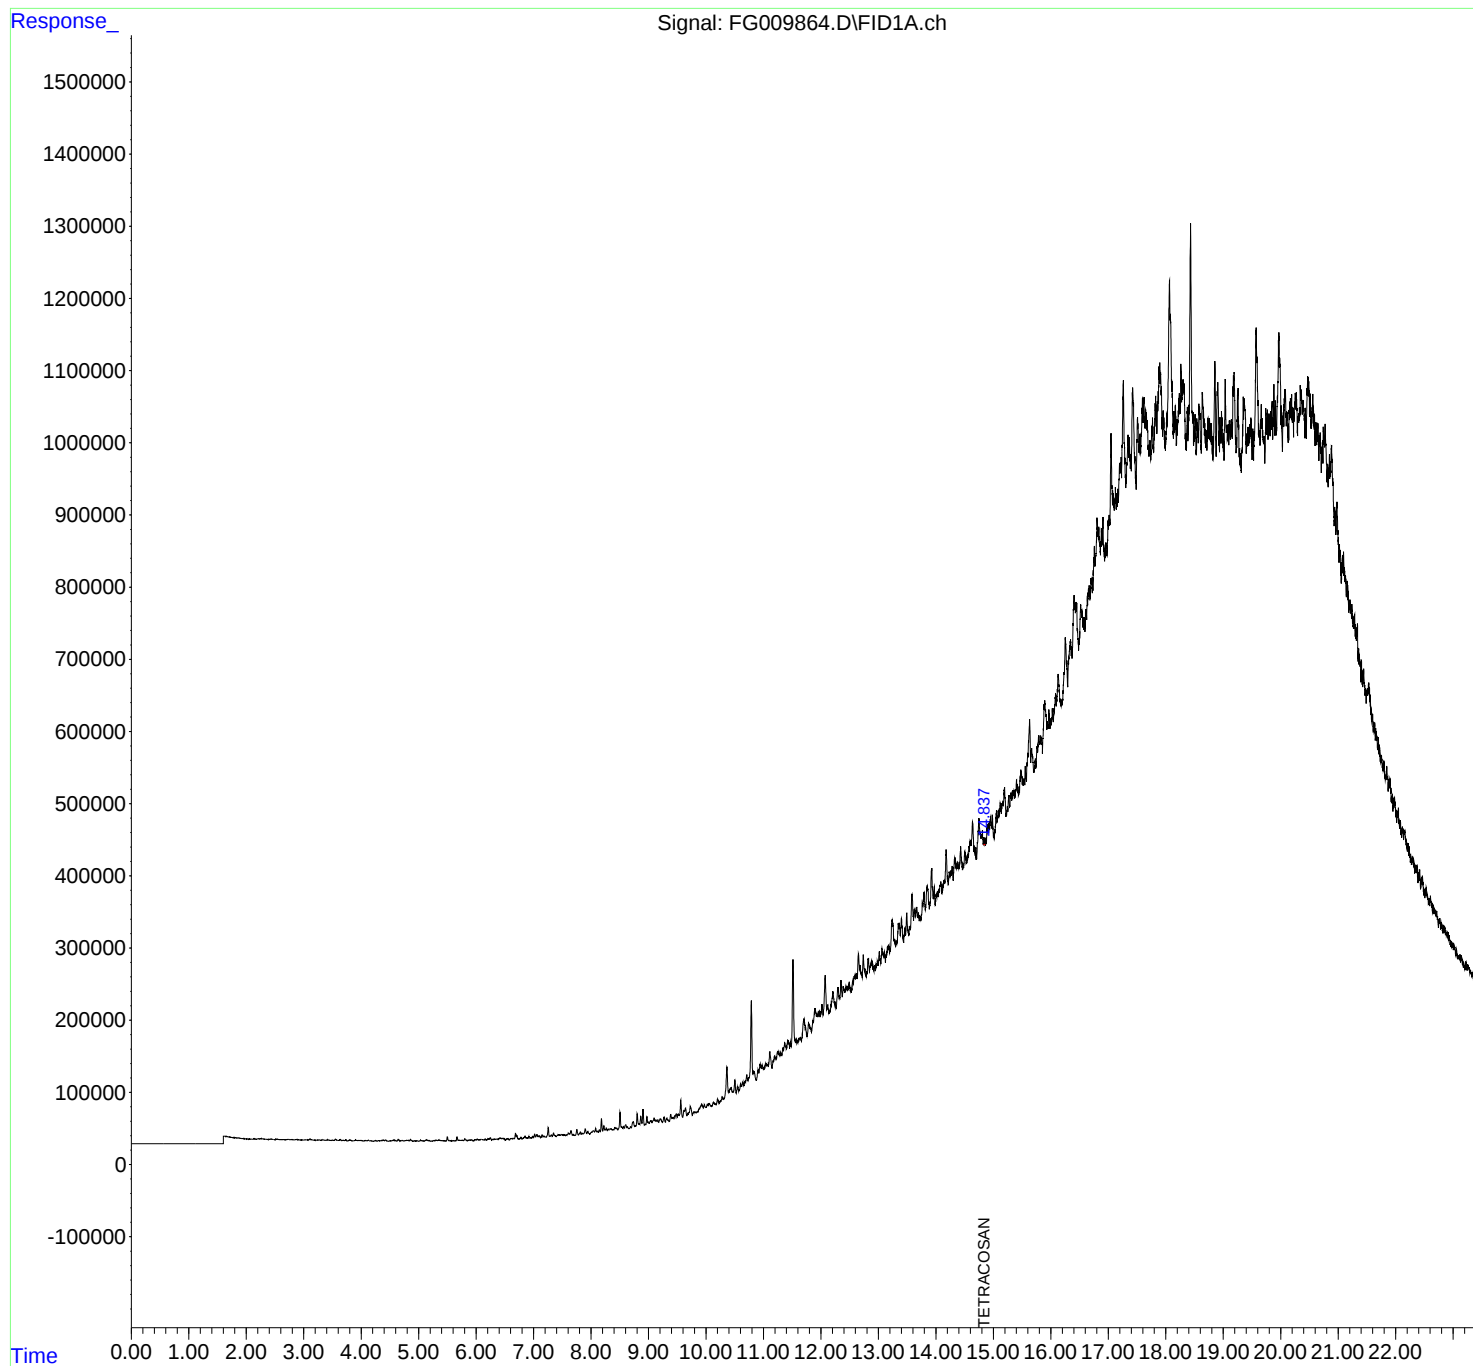

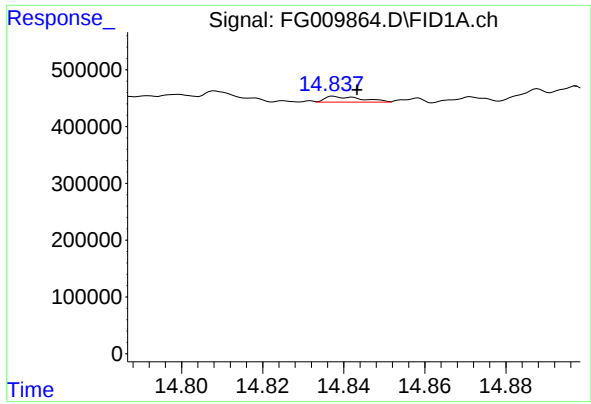

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.837 min
Delta R.T.: -0.006 min
Response: 63180
Conc: 0.60 ug/ml

Instrument :
FID_G
ClientSampleId :
WC-14A-1A-10-G

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022