

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061322\
Data File : FG009869.D
Signal(s) : FID1A.ch
Acq On : 13 Jun 2022 19:27
Operator : AJ\MA
Sample : N3328-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-02-061022

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

Integration File: autoint1.e
Quant Time: Jun 14 06:40:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.839	281917	2.678 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061322\
Data File : FG009869.D
Signal(s) : FID1A.ch
Acq On : 13 Jun 2022 19:27
Operator : AJ\MA
Sample : N3328-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
BU-02-061022


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

Integration File: autoint1.e
Quant Time: Jun 14 06:40:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

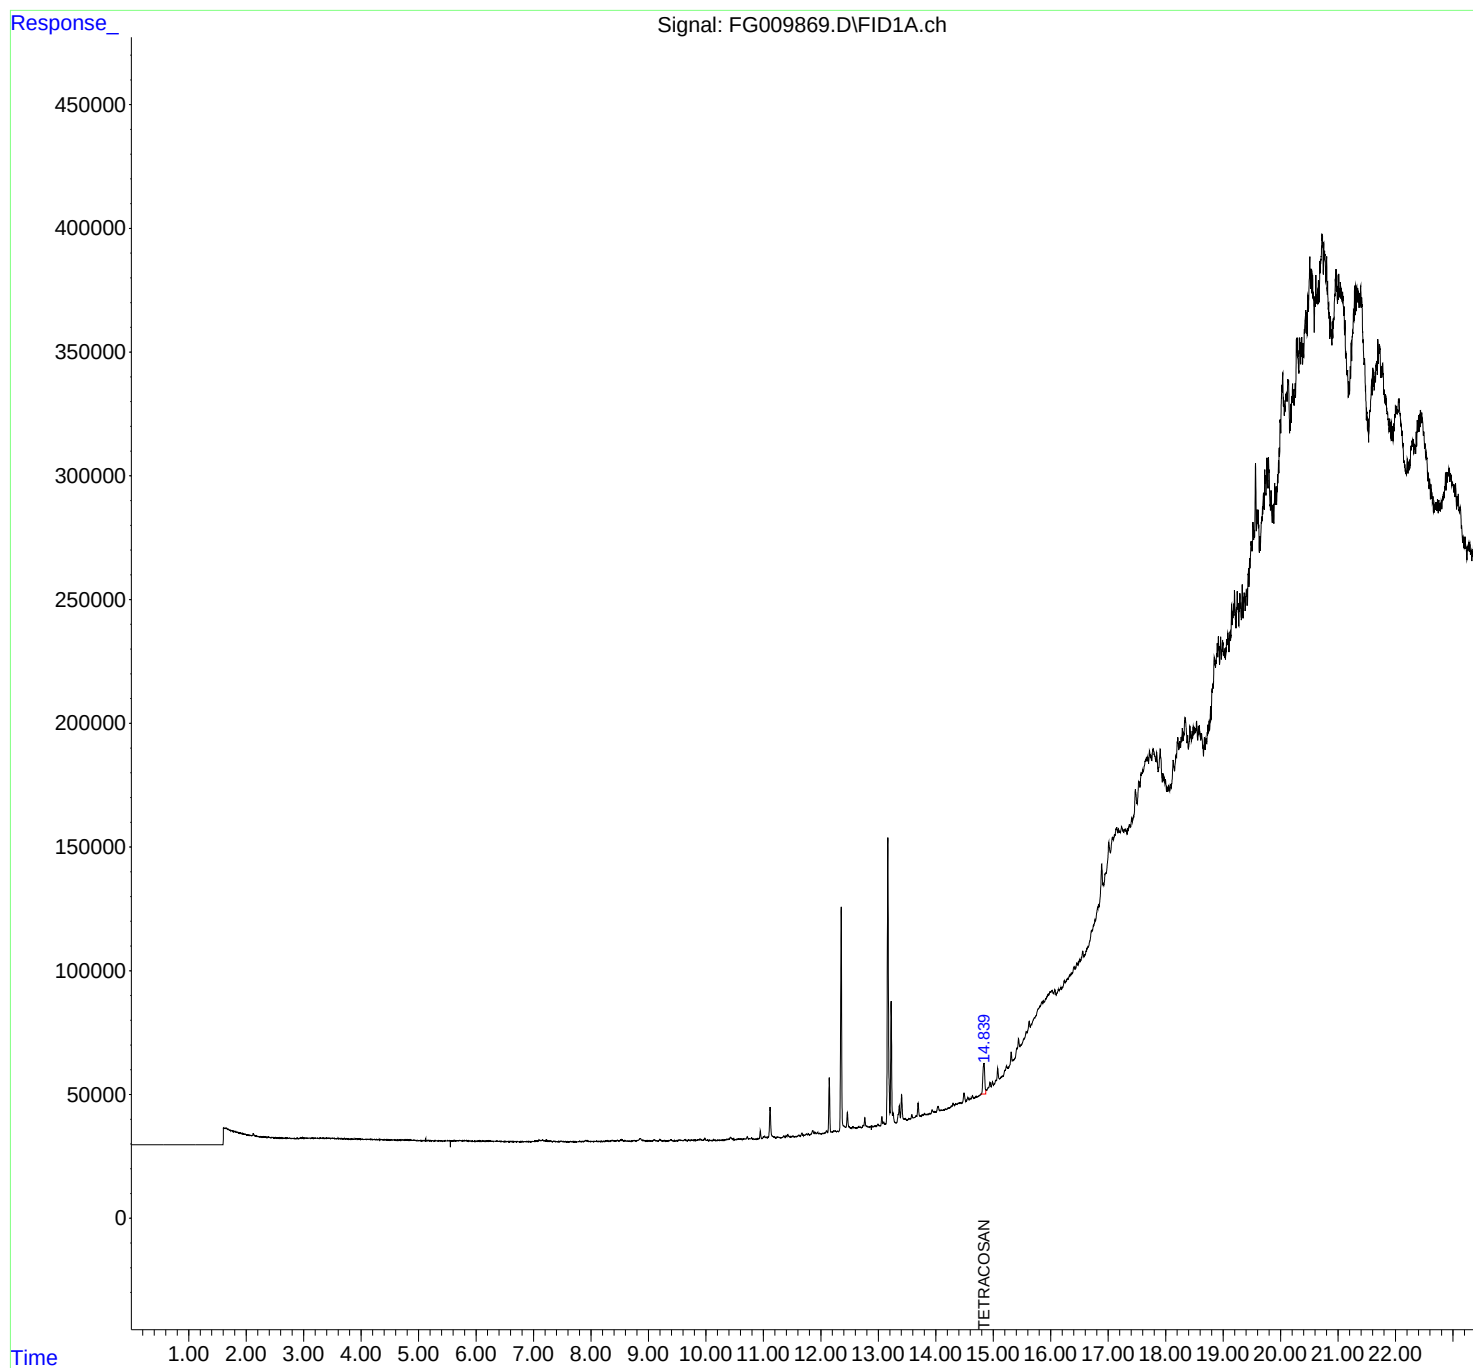

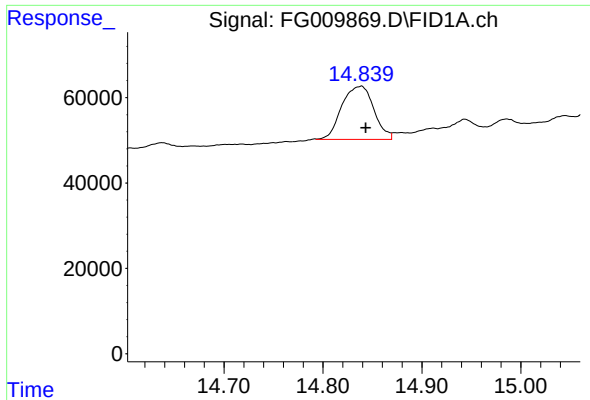

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.839 min
Delta R.T.: -0.004 min
Response: 281917
Conc: 2.68 ug/ml

Instrument :

FID_G

ClientSampleId :

BU-02-061022

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022