

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061323AL\
 Data File : FG012163.D
 Signal(s) : FID1A.ch
 Acq On : 13 Jun 2023 06:41
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 14 00:44:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 051923.M
 Quant Title : GC Extractables
 QLast Update : Fri May 19 12:59:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	17.906	20793	0.162 ug/ml
19) T n-Tetratriacontane (C34)	18.690	44275	0.361 ug/ml
20) T n-Hexatriacontane (C36)	19.438	95560	0.821 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061323AL\
Data File : FG012163.D
Signal(s) : FID1A.ch
Acq On : 13 Jun 2023 06:41
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 00:44:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 051923.M
Quant Title : GC Extractables
QLast Update : Fri May 19 12:59:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

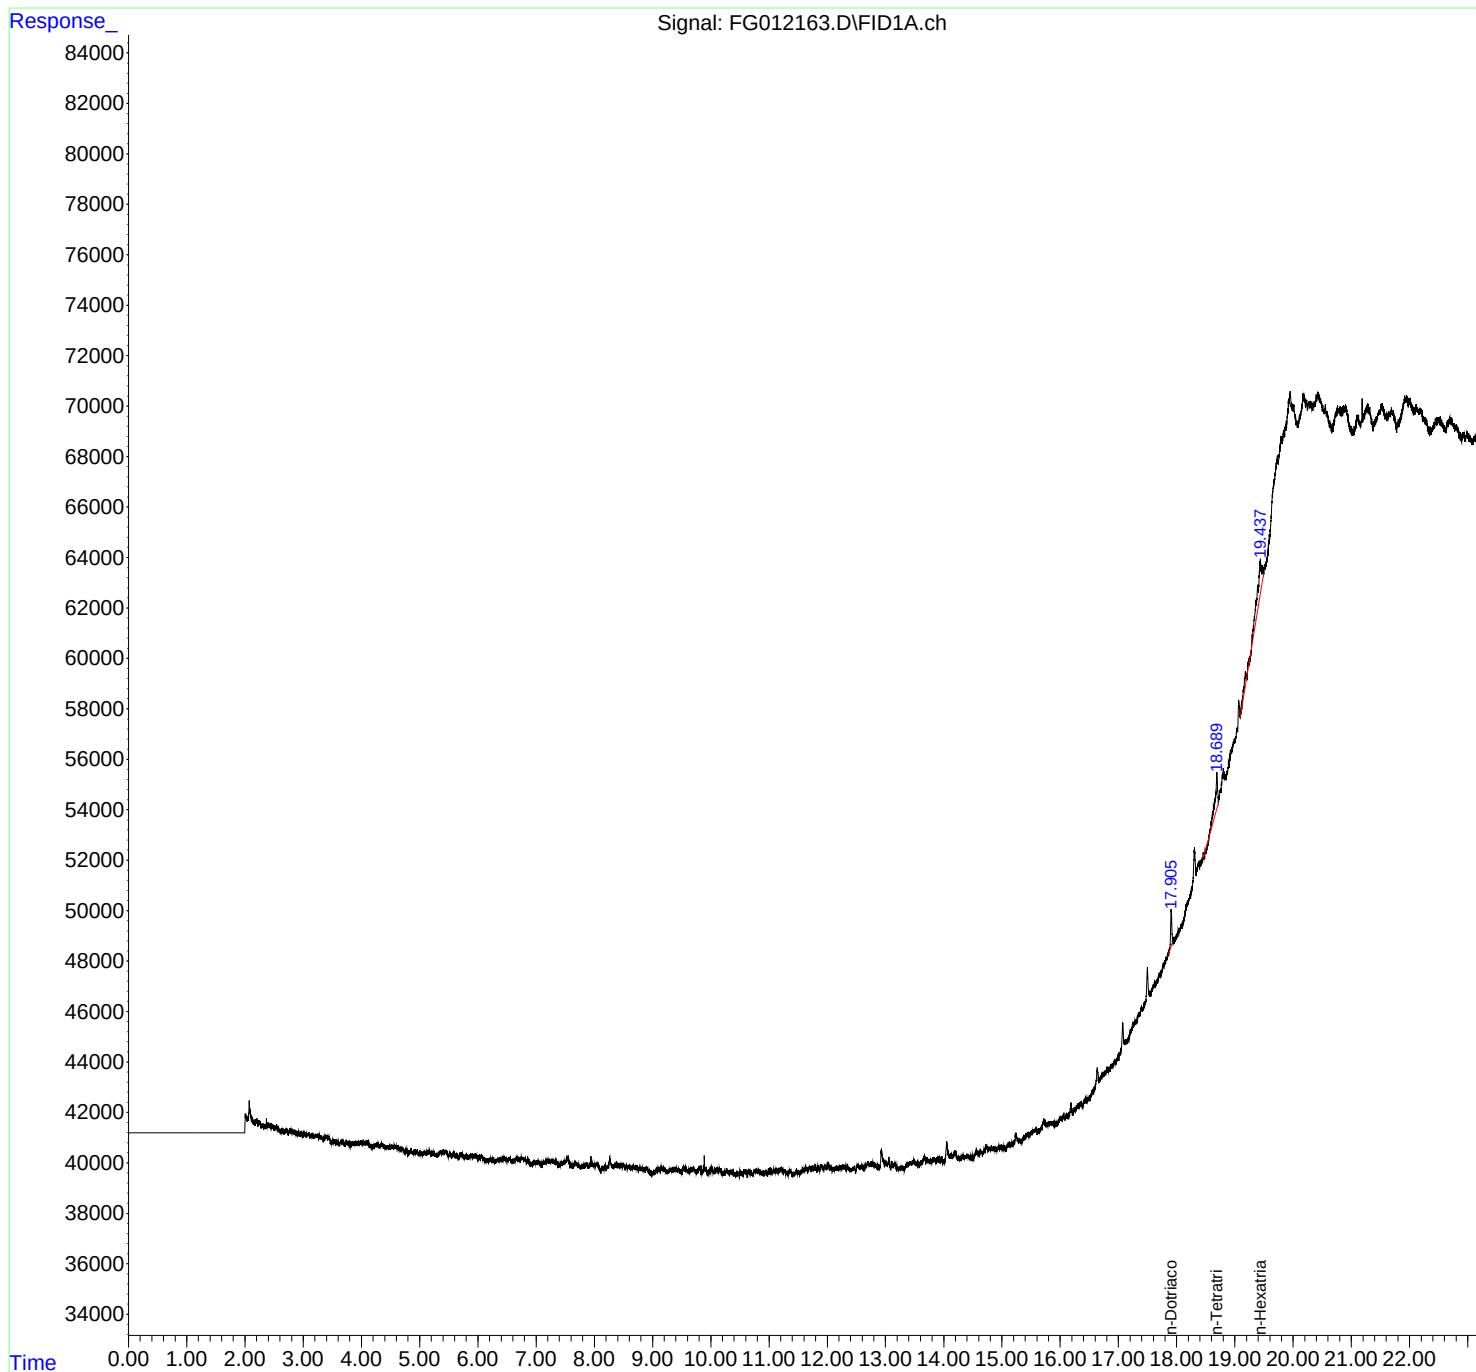


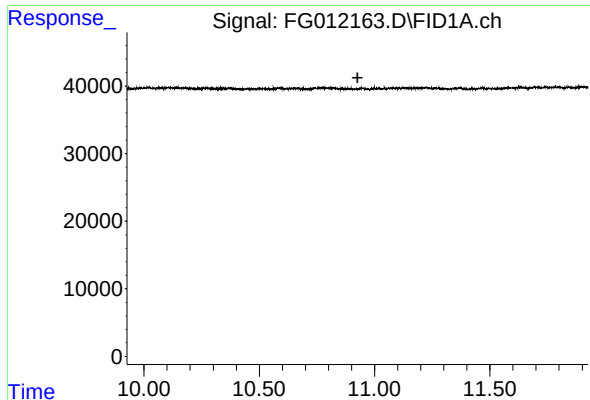

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 10.926 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

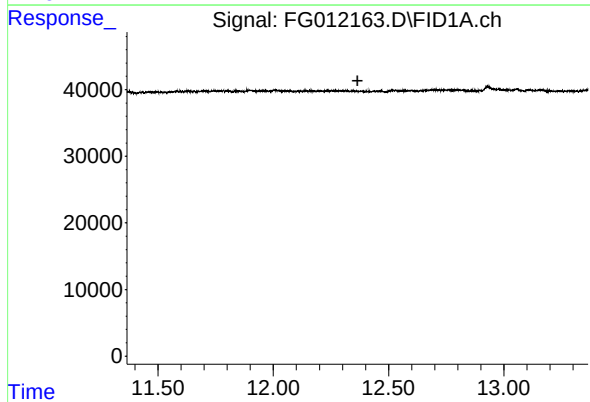


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.365 min
Response: 0
Conc: N.D.

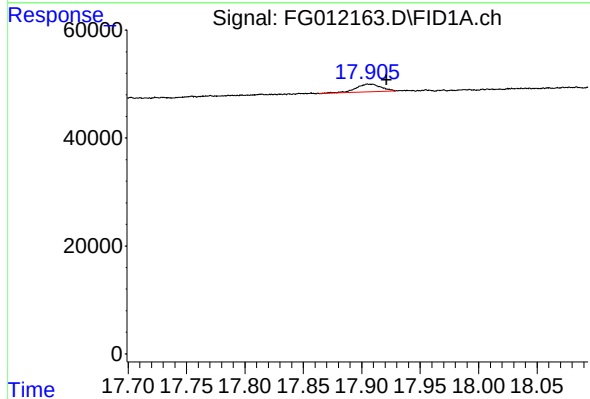


#18 n-Dotriacontane (C32)

R.T.: 17.906 min
Delta R.T.: -0.016 min
Response: 20793
Conc: 0.16 ug/ml

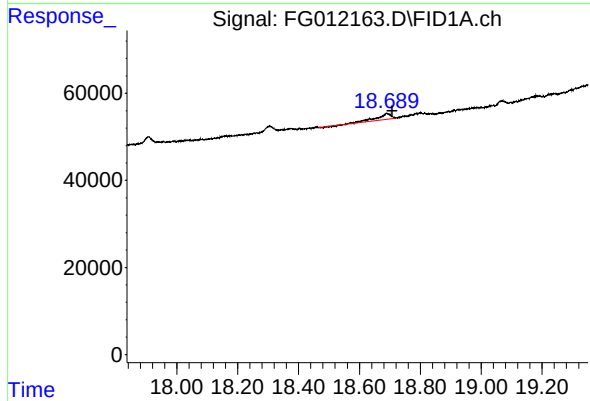

#19 n-Tetratriacontane (C34)

R.T.: 18.690 min
Delta R.T.: -0.018 min
Response: 44275
Conc: 0.36 ug/ml

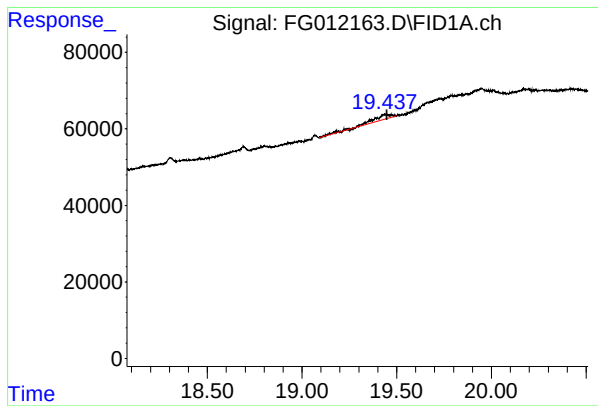

#20 n-Hexatriacontane (C36)

R.T.: 19.438 min
Delta R.T.: -0.011 min
Response: 95560
Conc: 0.82 ug/ml

Instrument :

FID_G

ClientSampleId :