

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061421\
Data File : FG008318.D
Signal(s) : FID1A.ch
Acq On : 14 Jun 2021 12:45
Operator : DD\AJ
Sample : M2674-02 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TMR-DS-02-060921

Manual Integrations
APPROVED

Ankita
6/15/2021 2:37:32 PM

Integration File: autoint1.e
Quant Time: Jun 15 01:19:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	346262	2.918 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061421\
Data File : FG008318.D
Signal(s) : FID1A.ch
Acq On : 14 Jun 2021 12:45
Operator : DD\AJ
Sample : M2674-02 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
TMR-DS-02-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:37:32 PM

Integration File: autoint1.e
Quant Time: Jun 15 01:19:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

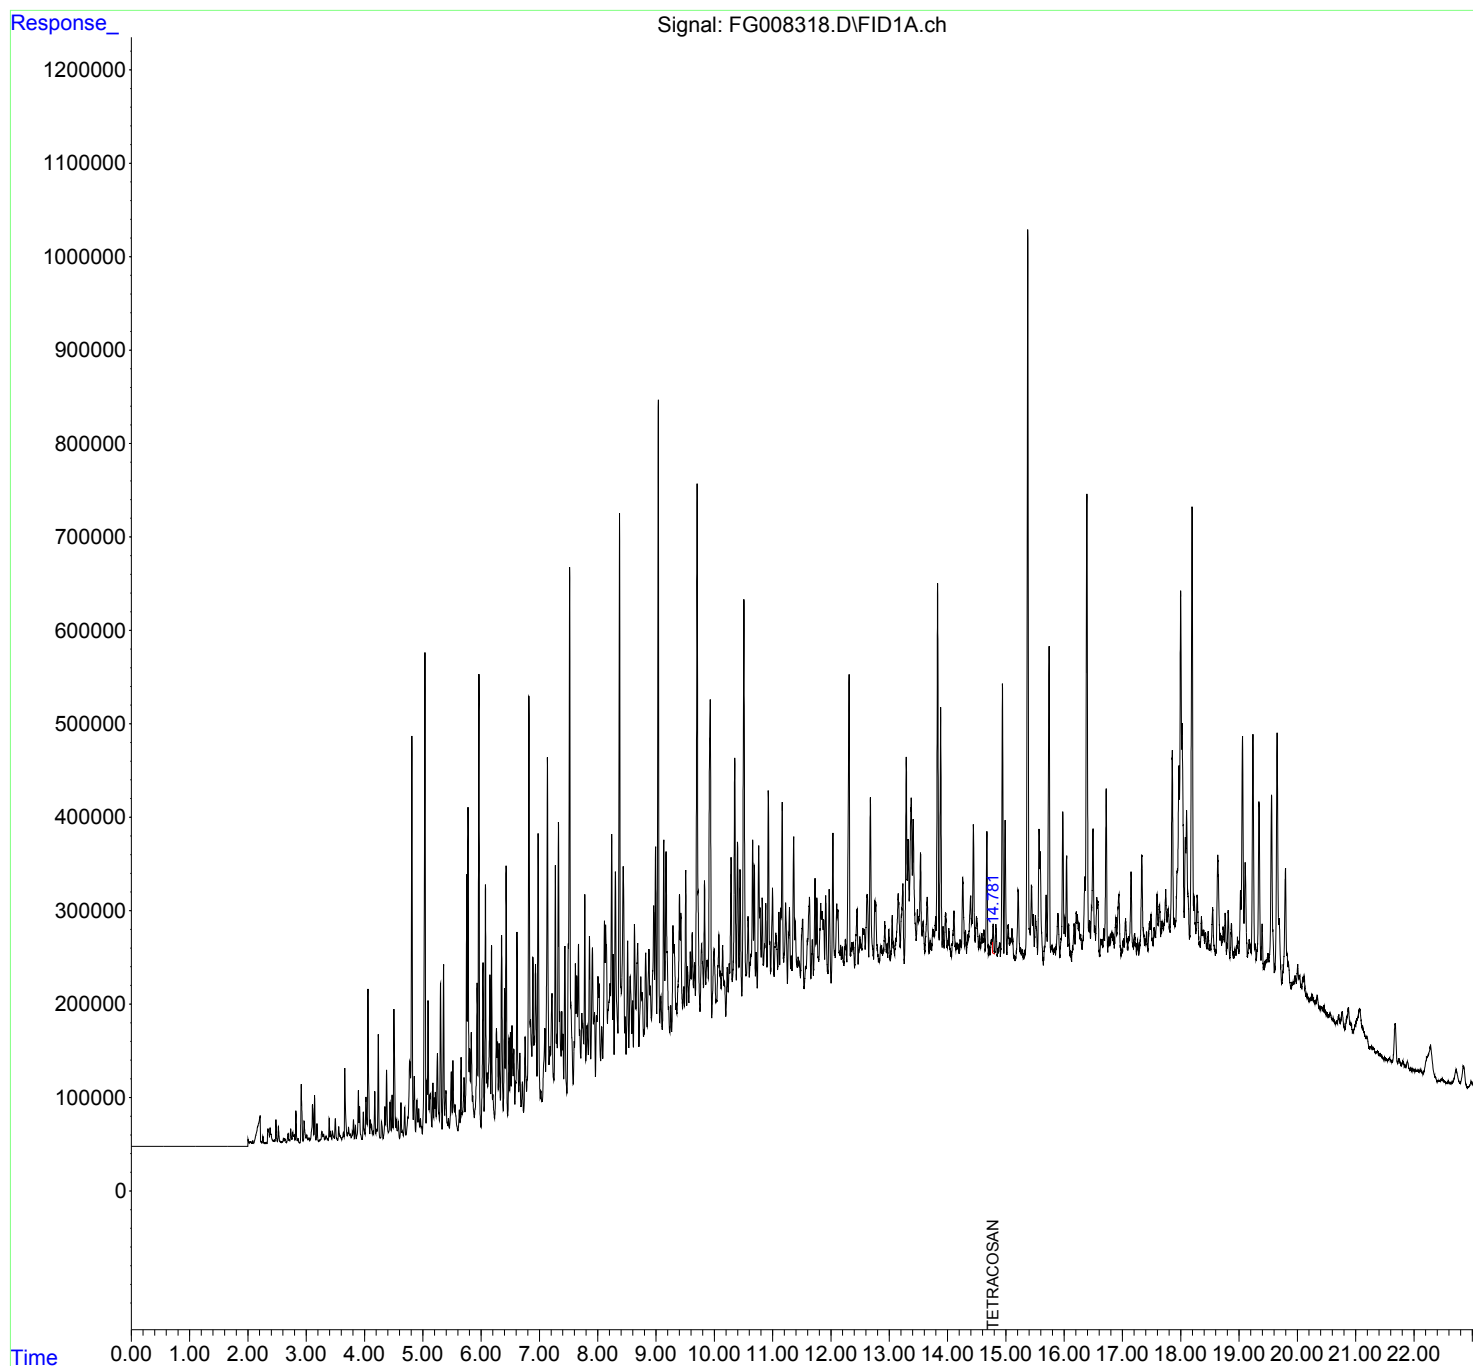

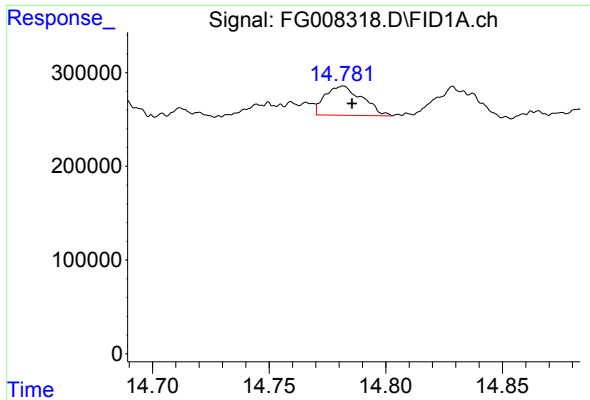

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.781 min
Delta R.T.: -0.004 min
Response: 346262
Conc: 2.92 ug/ml m

Instrument :
FID_G
ClientSampleId :
TMR-DS-02-060921

Manual Integrations
APPROVED

Ankita
6/15/2021 2:37:32 PM