

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061423\
 Data File : FG012177.D
 Signal(s) : FID1A.ch
 Acq On : 14 Jun 2023 15:02
 Operator : YP\AJ
 Sample : 03139-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 02:11:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
 Quant Title :
 QLast Update : Thu Jun 01 17:30:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.002	1554306	11.657 ug/ml
Target Compounds			
4) N-TETRADECANE	8.533	254354	1.698 ug/ml
6) N-OCTADECANE	11.610	263890	1.659 ug/ml
7) N-EICOSANE	12.964	348394	2.195 ug/ml
10) N-TETRACOSANE	15.251	187216	1.253 ug/ml
12) N-OCTACOSANE	17.228	177011	1.308 ug/ml
13) N-TRIACONTANE	18.070	368537	2.781 ug/ml
14) N-DOTRIACONTANE	18.901	875964	6.862 ug/ml
15) N-TETRATRIACONTANE	19.718	402423	3.306 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061423\
Data File : FG012177.D
Signal(s) : FID1A.ch
Acq On : 14 Jun 2023 15:02
Operator : YP\AJ
Sample : 03139-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 02:11:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

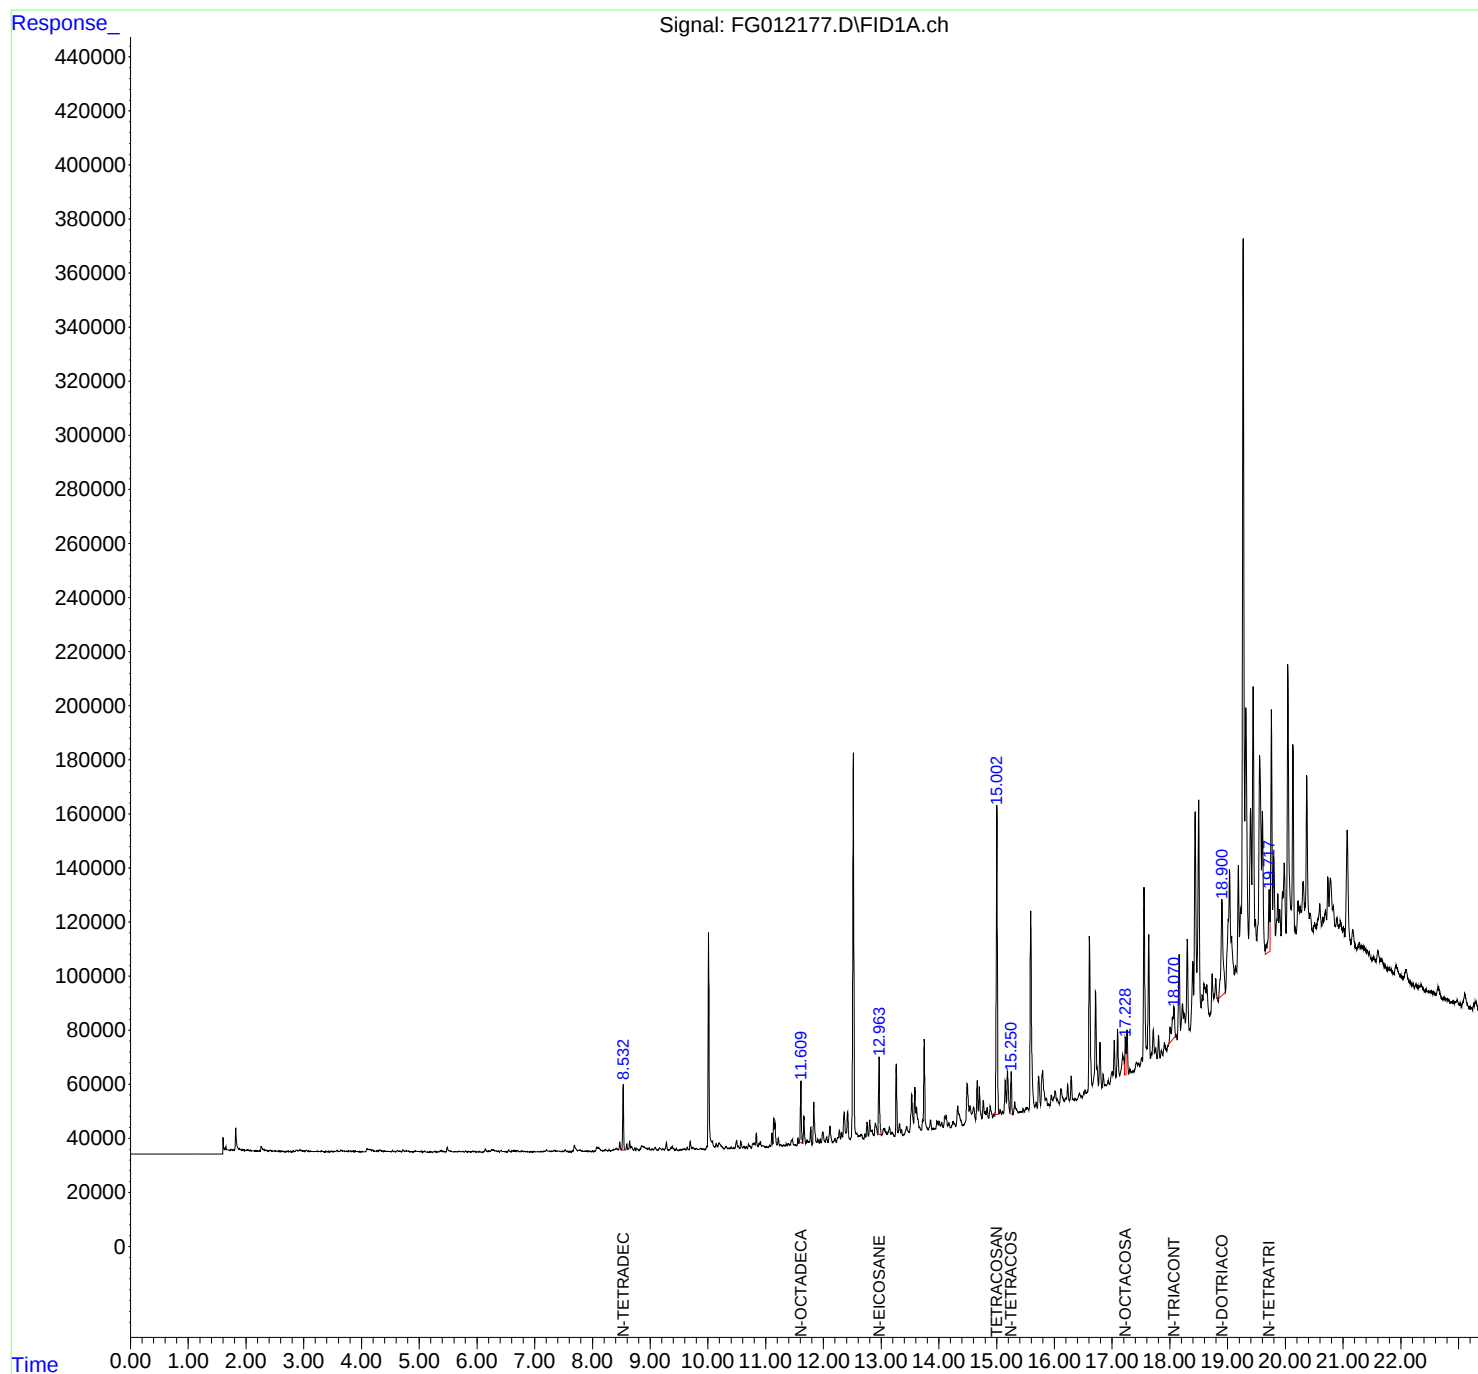


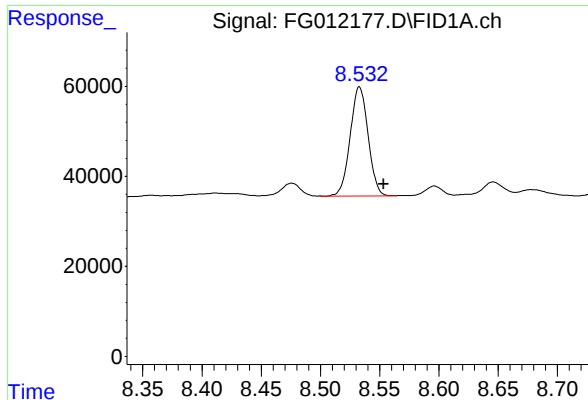

#4 N-TETRADECANE


R.T.: 8.533 min
Delta R.T.: -0.021 min
Response: 254354
Conc: 1.70 ug/ml

Instrument :
FID_G
ClientSampleId :

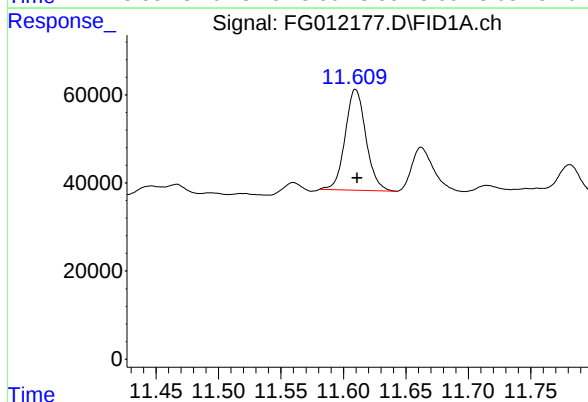


#6 N-OCTADECANE

R.T.: 11.610 min
Delta R.T.: -0.002 min
Response: 263890
Conc: 1.66 ug/ml

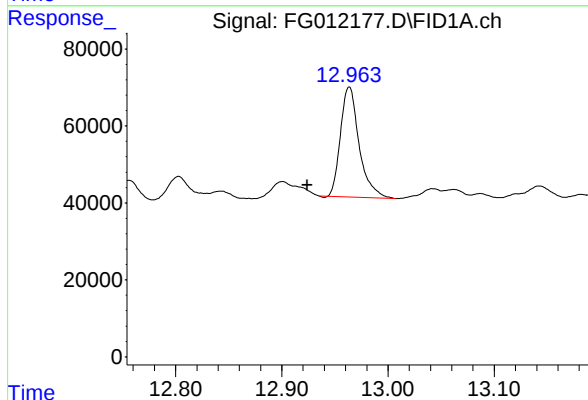


#7 N-EICOSANE

R.T.: 12.964 min
Delta R.T.: 0.040 min
Response: 348394
Conc: 2.20 ug/ml

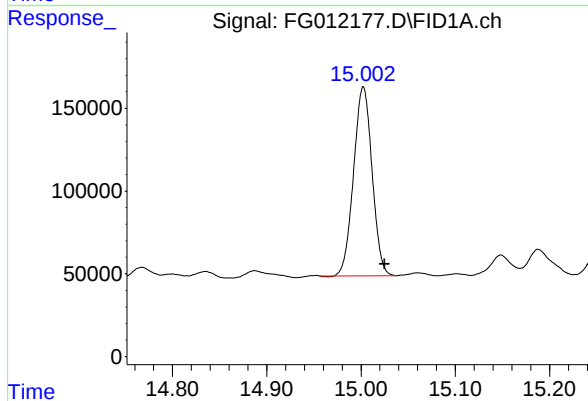

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.002 min
Delta R.T.: -0.023 min
Response: 1554306
Conc: 11.66 ug/ml

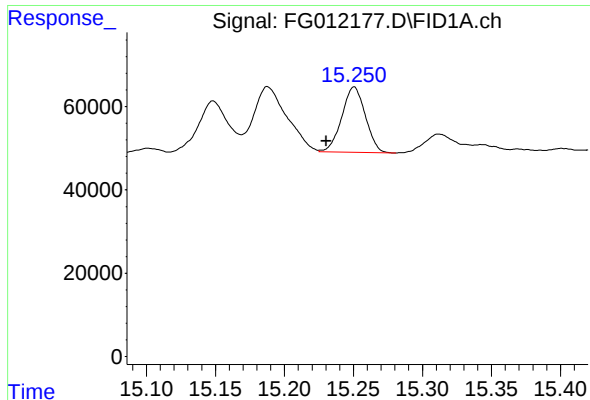

#10 N-TETRACOSANE


R.T.: 15.251 min
Delta R.T.: 0.020 min
Response: 187216
Conc: 1.25 ug/ml

Instrument :
FID_G
ClientSampleId :

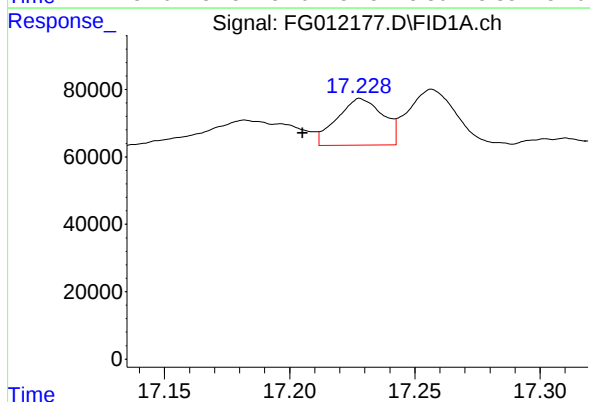


#12 N-OCTACOSANE

R.T.: 17.228 min
Delta R.T.: 0.023 min
Response: 177011
Conc: 1.31 ug/ml

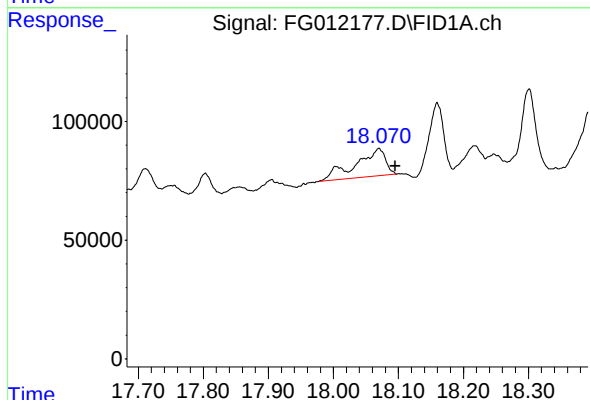


#13 N-TRIACONTANE

R.T.: 18.070 min
Delta R.T.: -0.025 min
Response: 368537
Conc: 2.78 ug/ml

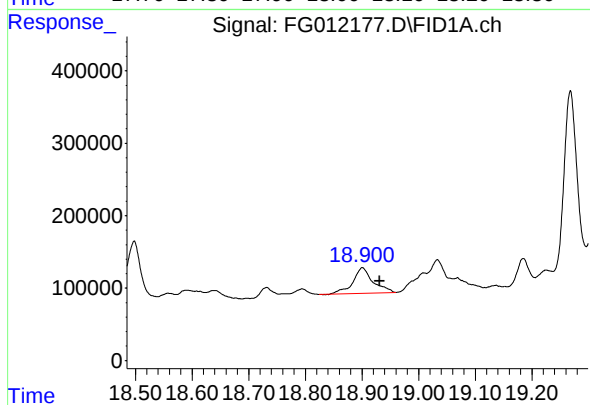

#14 N-DOTRIACONTANE

R.T.: 18.901 min
Delta R.T.: -0.030 min
Response: 875964
Conc: 6.86 ug/ml

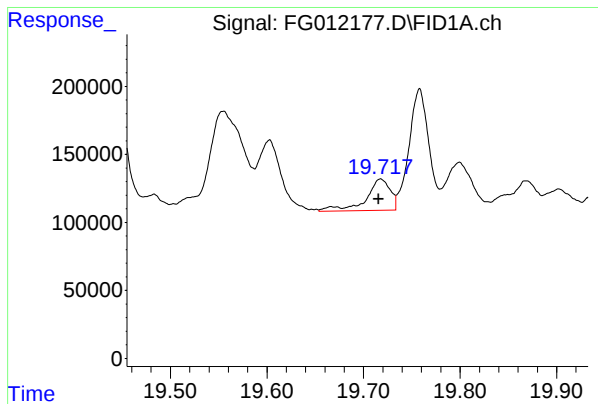

#15 N-TETRATRIACONTANE

R.T.: 19.718 min
Delta R.T.: 0.002 min
Response: 402423
Conc: 3.31 ug/ml

Instrument :
FID_G
ClientSampleId :