

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061423\
Data File : FG012175.D
Signal(s) : FID1A.ch
Acq On : 14 Jun 2023 14:03
Operator : YP\AJ
Sample : PB153427BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB153427BL

Integration File: autoint1.e
Quant Time: Jun 15 02:11:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.006	2115192	15.864 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061423\
Data File : FG012175.D
Signal(s) : FID1A.ch
Acq On : 14 Jun 2023 14:03
Operator : YP\AJ
Sample : PB153427BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB153427BL

Integration File: autoint1.e
Quant Time: Jun 15 02:11:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

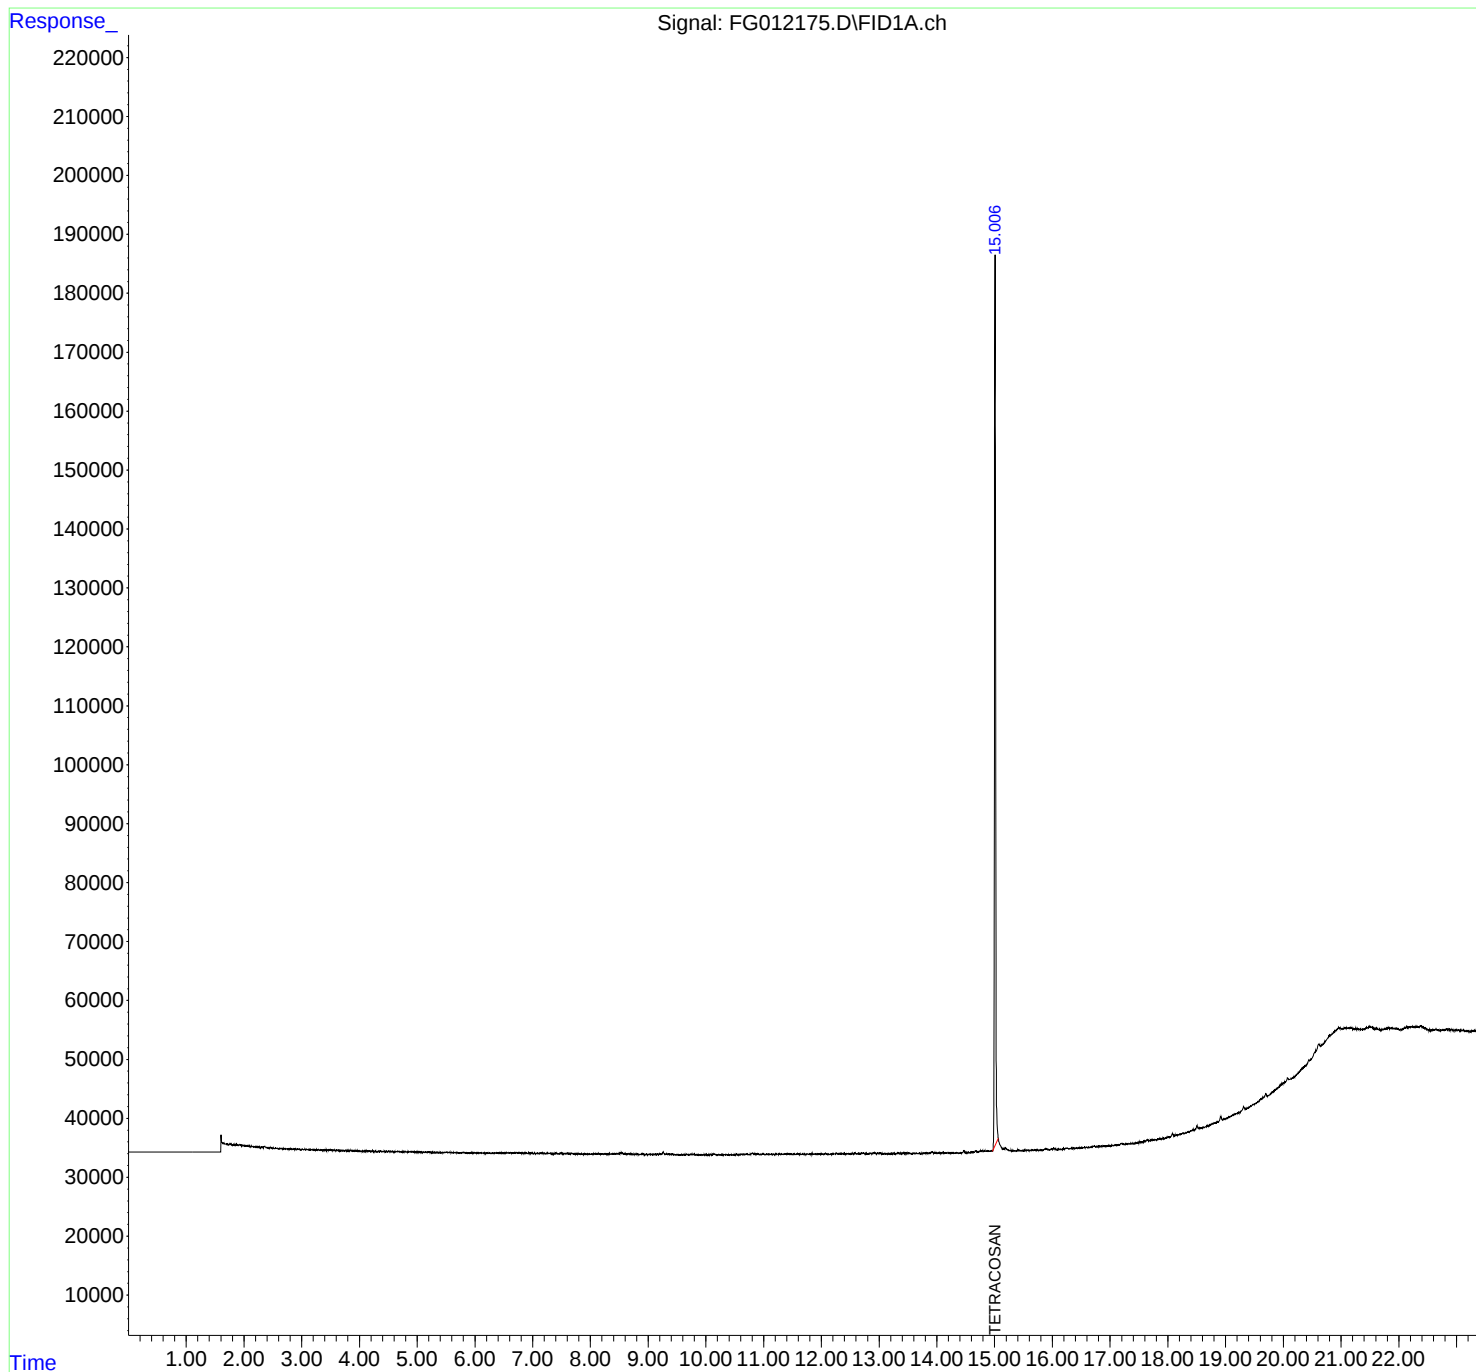

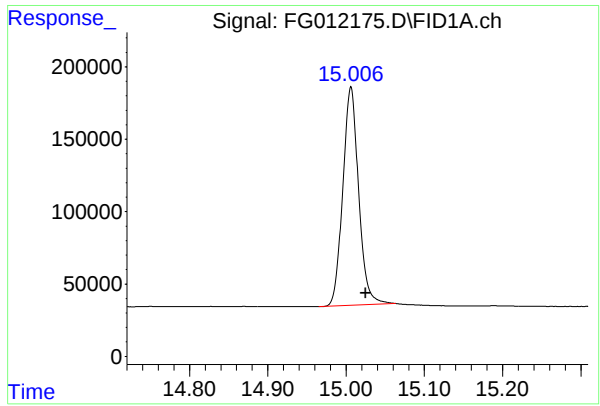

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.006 min
Delta R.T.: -0.019 min
Response: 2115192
Conc: 15.86 ug/ml

Instrument :
FID_G
ClientSampleId :
PB153427BL