

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
 Data File : FF008626.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2021 12:13
 Operator : DD\AJ
 Sample : M2674-01 300X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 13:12:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
2) N-DECANE	4.545	96201	0.793 ug/ml
3) N-DODECANE	6.573	69581	0.558 ug/ml
4) N-TETRADECANE	8.366	754009	5.925 ug/ml
5) N-HEXADECANE	9.905	171782	1.359 ug/ml
8) N-DOCOSANE	13.852	102891	0.818 ug/ml
10) N-TETRACOSANE	14.953	96908	0.791 ug/ml
13) N-TRIACONTANE	17.806	125235	1.057 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008626.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 12:13
Operator : DD\AJ
Sample : M2674-01 300X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 13:12:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

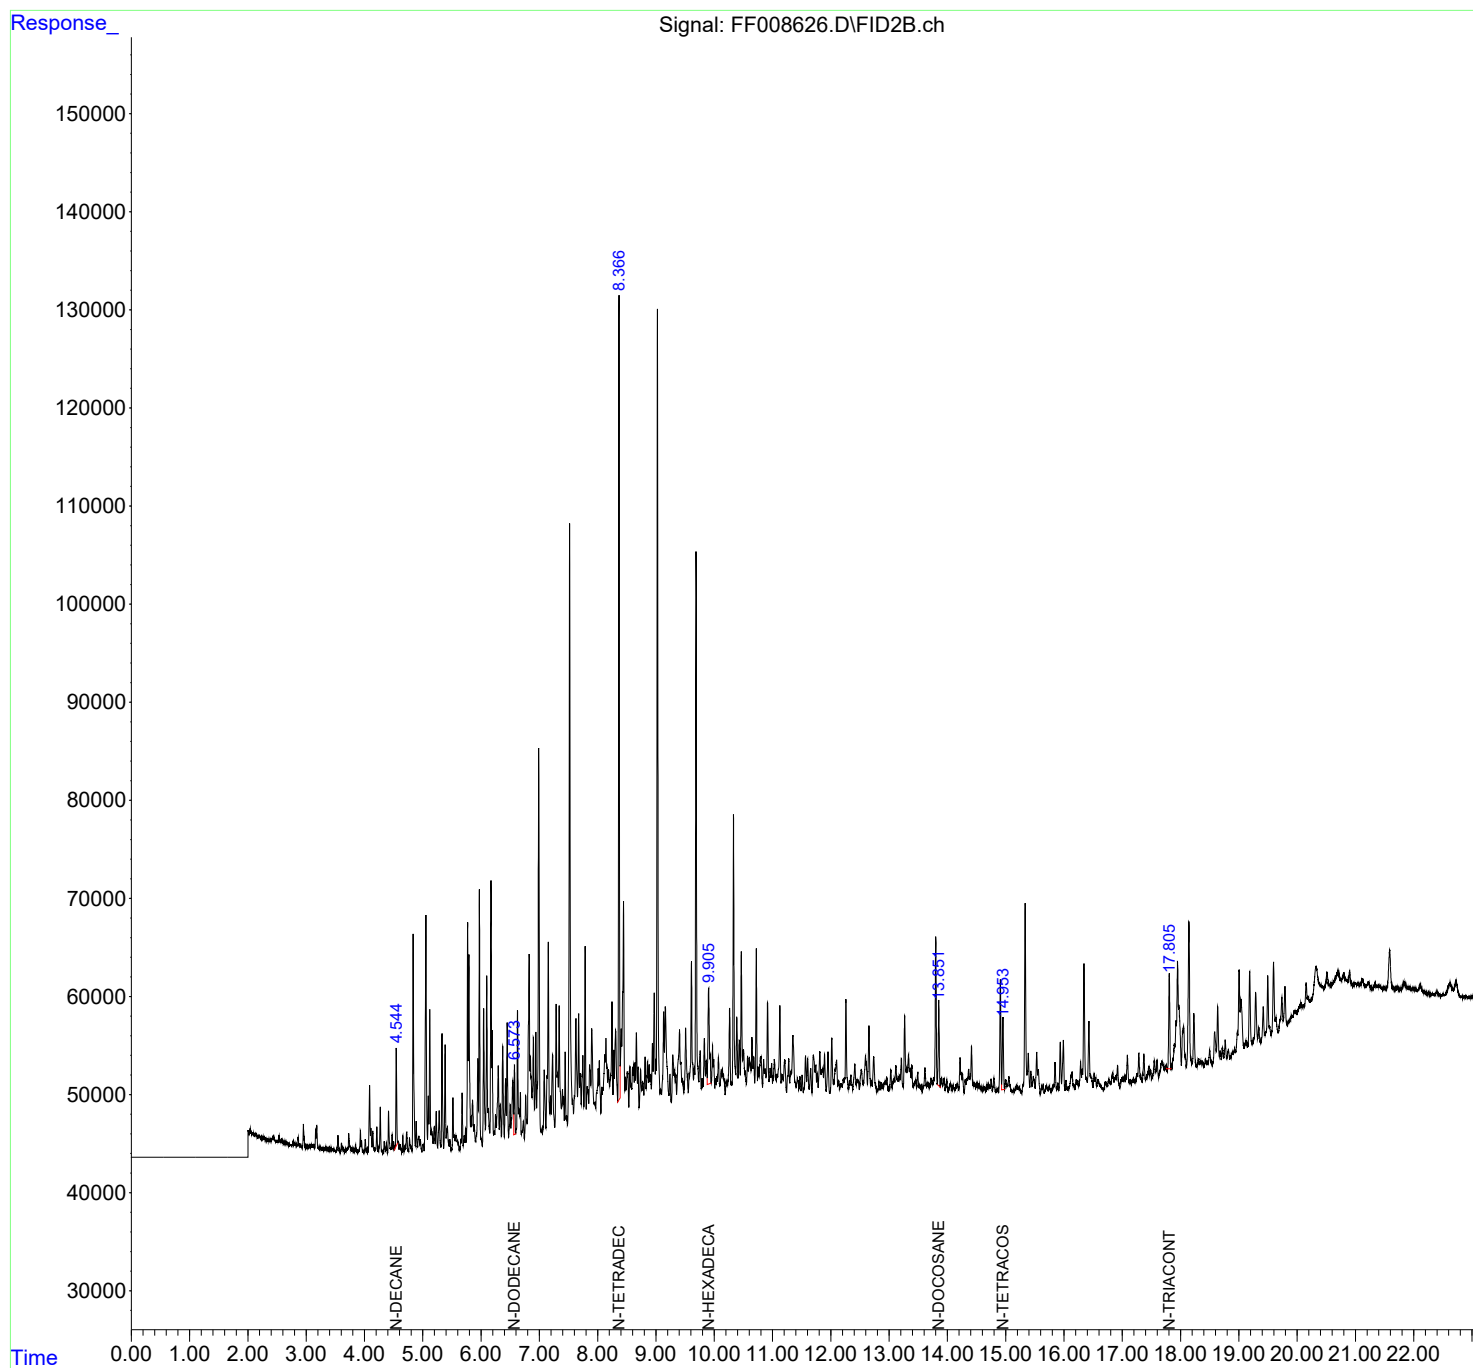


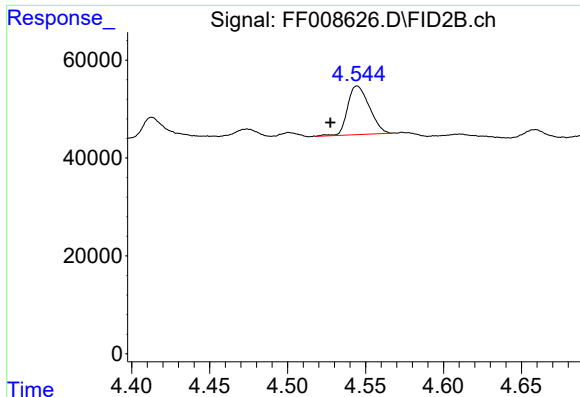

#2 N-DECANE


R.T.: 4.545 min
Delta R.T.: 0.017 min
Response: 96201
Conc: 0.79 ug/ml

Instrument :
FID_G
ClientSampleId :

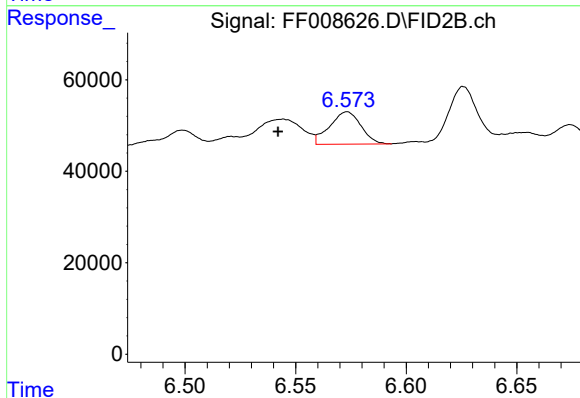


#3 N-DODECANE

R.T.: 6.573 min
Delta R.T.: 0.031 min
Response: 69581
Conc: 0.56 ug/ml

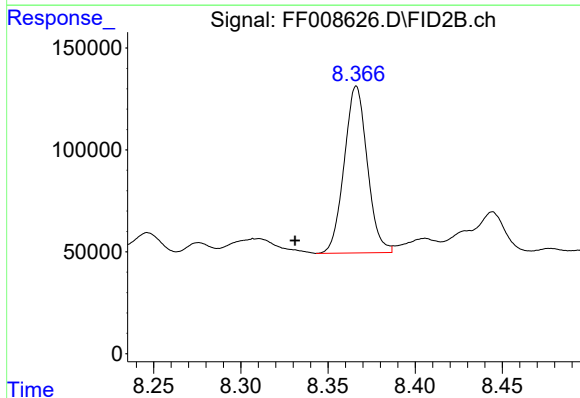


#4 N-TETRADECANE

R.T.: 8.366 min
Delta R.T.: 0.035 min
Response: 754009
Conc: 5.92 ug/ml

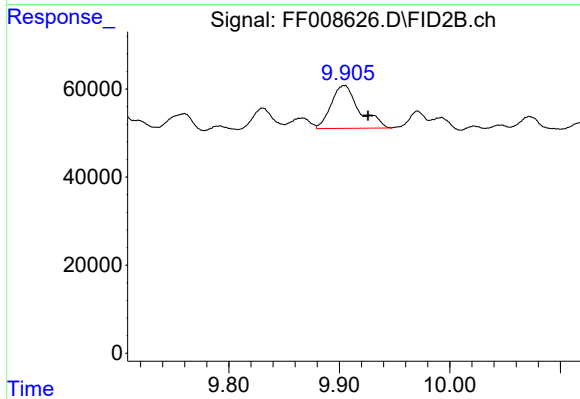

#5 N-HEXADECANE


R.T.: 9.905 min
Delta R.T.: -0.021 min
Response: 171782
Conc: 1.36 ug/ml

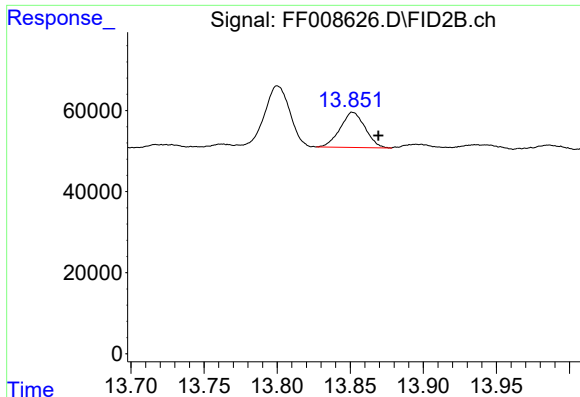

#8 N-DOCOSANE


R.T.: 13.852 min
Delta R.T.: -0.018 min
Response: 102891
Conc: 0.82 ug/ml

Instrument :
FID_G
ClientSampleId :

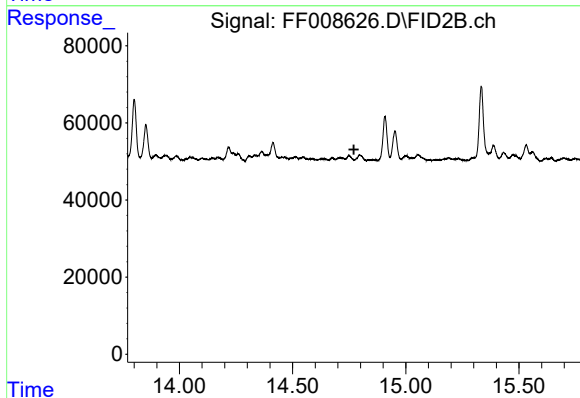


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.771 min
Response: 0
Conc: N.D.

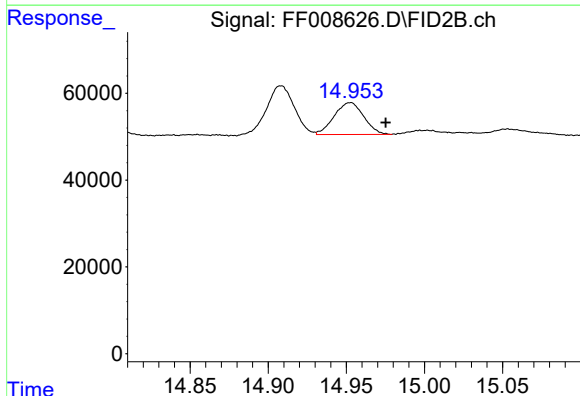

#10 N-TETRACOSANE

R.T.: 14.953 min
Delta R.T.: -0.023 min
Response: 96908
Conc: 0.79 ug/ml

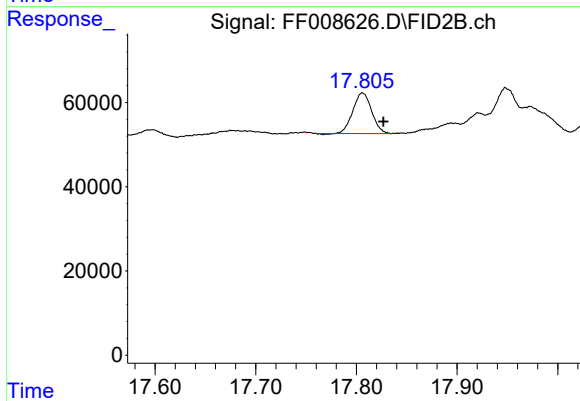

#13 N-TRIACONTANE

R.T.: 17.806 min
Delta R.T.: -0.021 min
Response: 125235
Conc: 1.06 ug/ml