

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061521\
 Data File : FG008334.D
 Signal(s) : FID1A.ch
 Acq On : 15 Jun 2021 15:53
 Operator : DD\AJ
 Sample : M2672-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 16 02:20:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.775	1130789	9.528 ug/ml
Target Compounds			
8) N-DOCOSANE	13.871	80637	0.594 ug/ml
10) N-TETRACOSANE	14.967	271834	2.021 ug/ml
11) N-HEXACOSANE	16.004	116943	0.890 ug/ml
12) N-OCTACOSANE	16.956	112643	0.869 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061521\
Data File : FG008334.D
Signal(s) : FID1A.ch
Acq On : 15 Jun 2021 15:53
Operator : DD\AJ
Sample : M2672-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:20:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

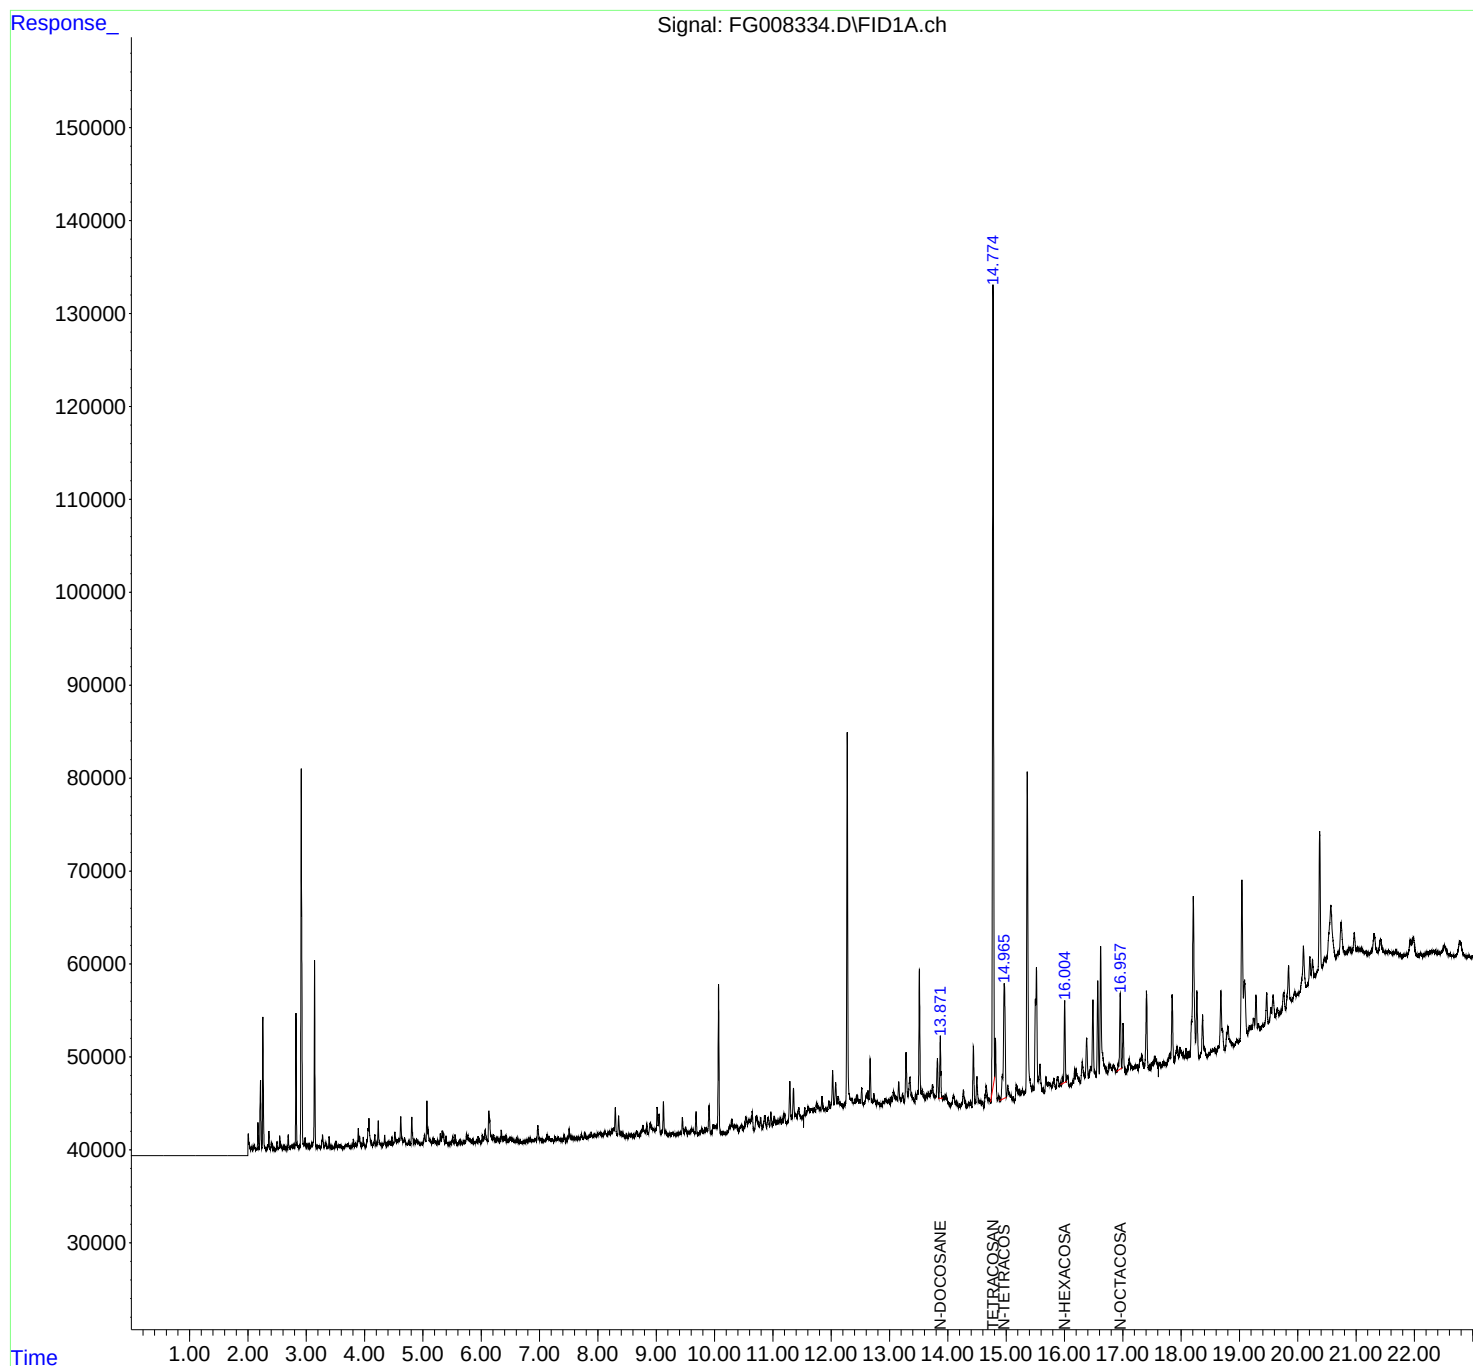


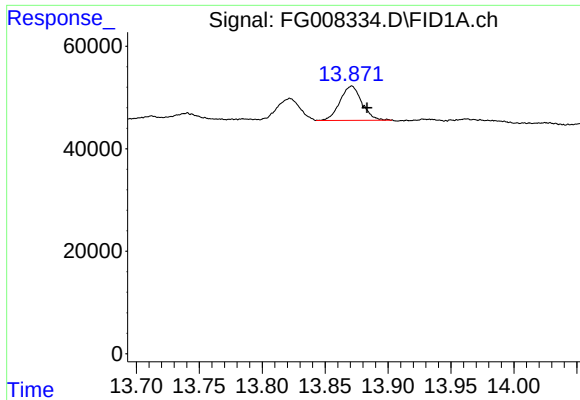

#8 N-DOCOSANE


R.T.: 13.871 min
Delta R.T.: -0.012 min
Response: 80637
Conc: 0.59 ug/ml

Instrument :
FID_G
ClientSampleId :

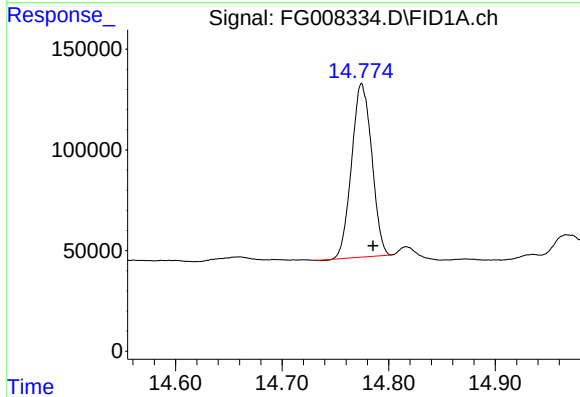


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.775 min
Delta R.T.: -0.011 min
Response: 1130789
Conc: 9.53 ug/ml

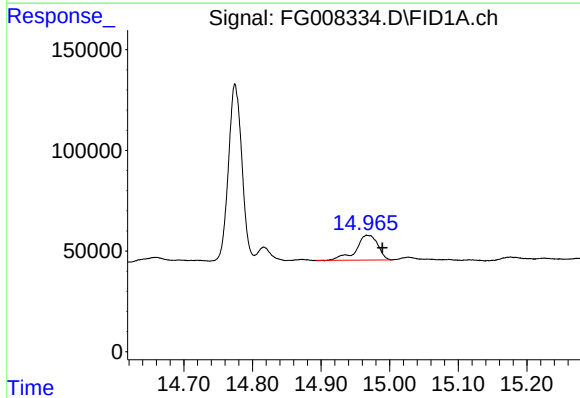


#10 N-TETRACOSANE

R.T.: 14.967 min
Delta R.T.: -0.022 min
Response: 271834
Conc: 2.02 ug/ml

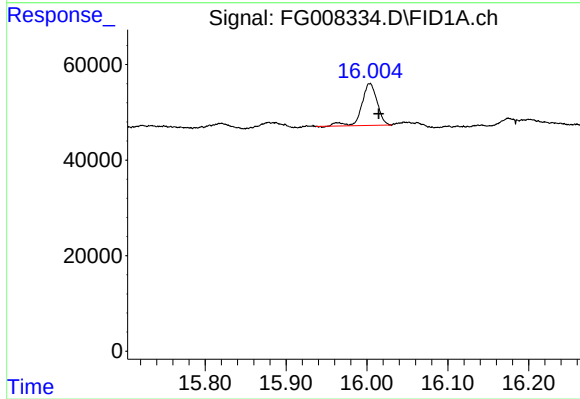

#11 N-HEXACOSANE

R.T.: 16.004 min
Delta R.T.: -0.011 min
Response: 116943
Conc: 0.89 ug/ml

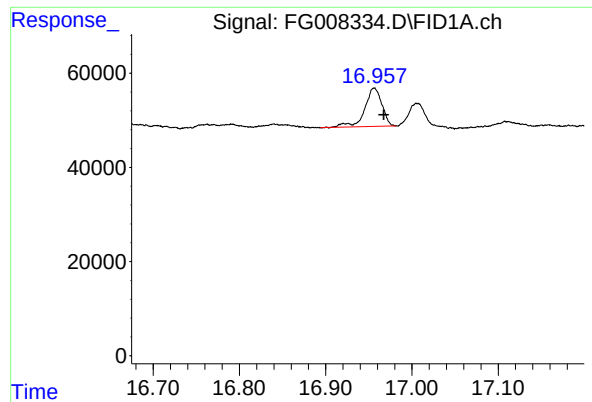

#12 N-OCTACOSANE

R.T.: 16.956 min
Delta R.T.: -0.011 min
Response: 112643
Conc: 0.87 ug/ml

Instrument :
FID_G
ClientSampleId :