

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061521\
Data File : FG008339.D
Signal(s) : FID1A.ch
Acq On : 15 Jun 2021 18:31
Operator : DD\AJ
Sample : M2672-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:21:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.775	1475779	12.436 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.005	99400	0.767 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061521\
Data File : FG008339.D
Signal(s) : FID1A.ch
Acq On : 15 Jun 2021 18:31
Operator : DD\AJ
Sample : M2672-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:21:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

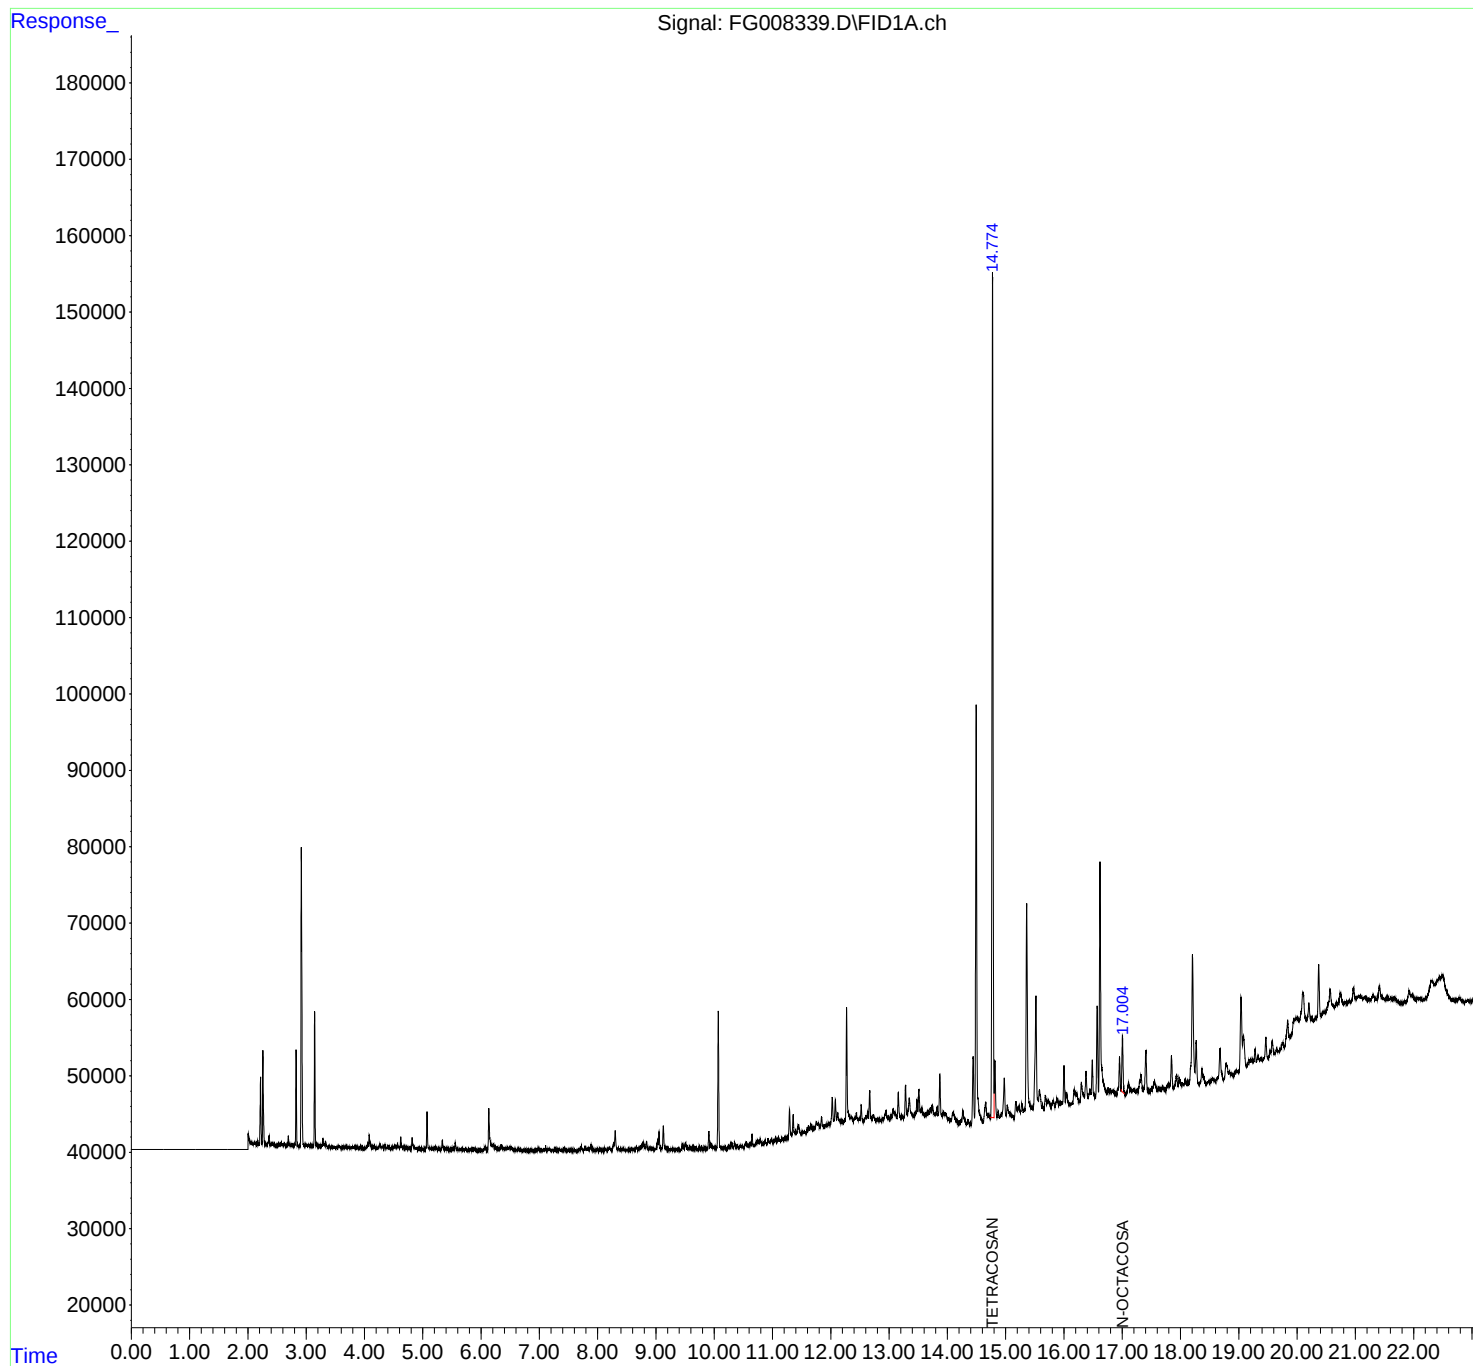


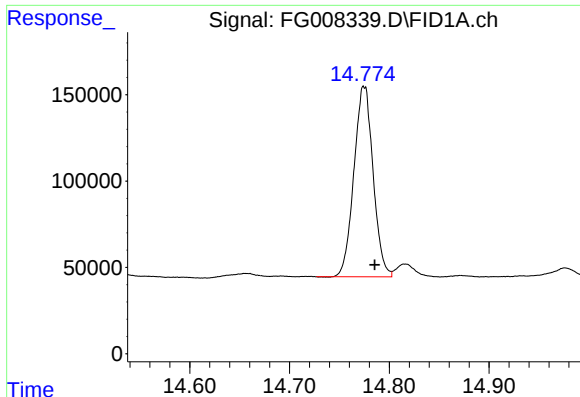

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.775 min
Delta R.T.: -0.011 min
Response: 1475779
Conc: 12.44 ug/ml

Instrument :
FID_G
ClientSampleId :

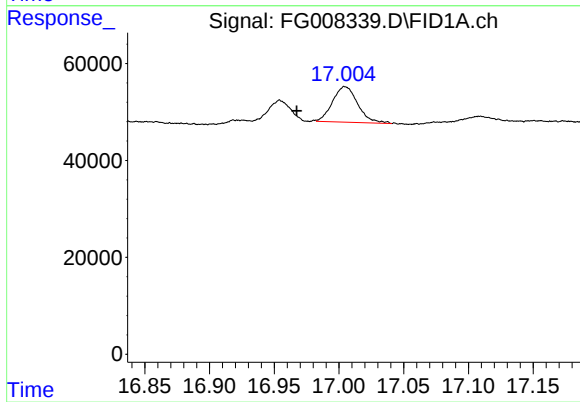

#12 N-OCTACOSANE

R.T.: 17.005 min
Delta R.T.: 0.037 min
Response: 99400
Conc: 0.77 ug/ml