

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061521\
Data File : FG008343.D
Signal(s) : FID1A.ch
Acq On : 15 Jun 2021 20:38
Operator : DD\AJ
Sample : M2672-20
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:21:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.775	1959074	16.508 ug/ml
Target Compounds			
8) N-DOCOSANE	13.870	90108	0.664 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061521\
Data File : FG008343.D
Signal(s) : FID1A.ch
Acq On : 15 Jun 2021 20:38
Operator : DD\AJ
Sample : M2672-20
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:21:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

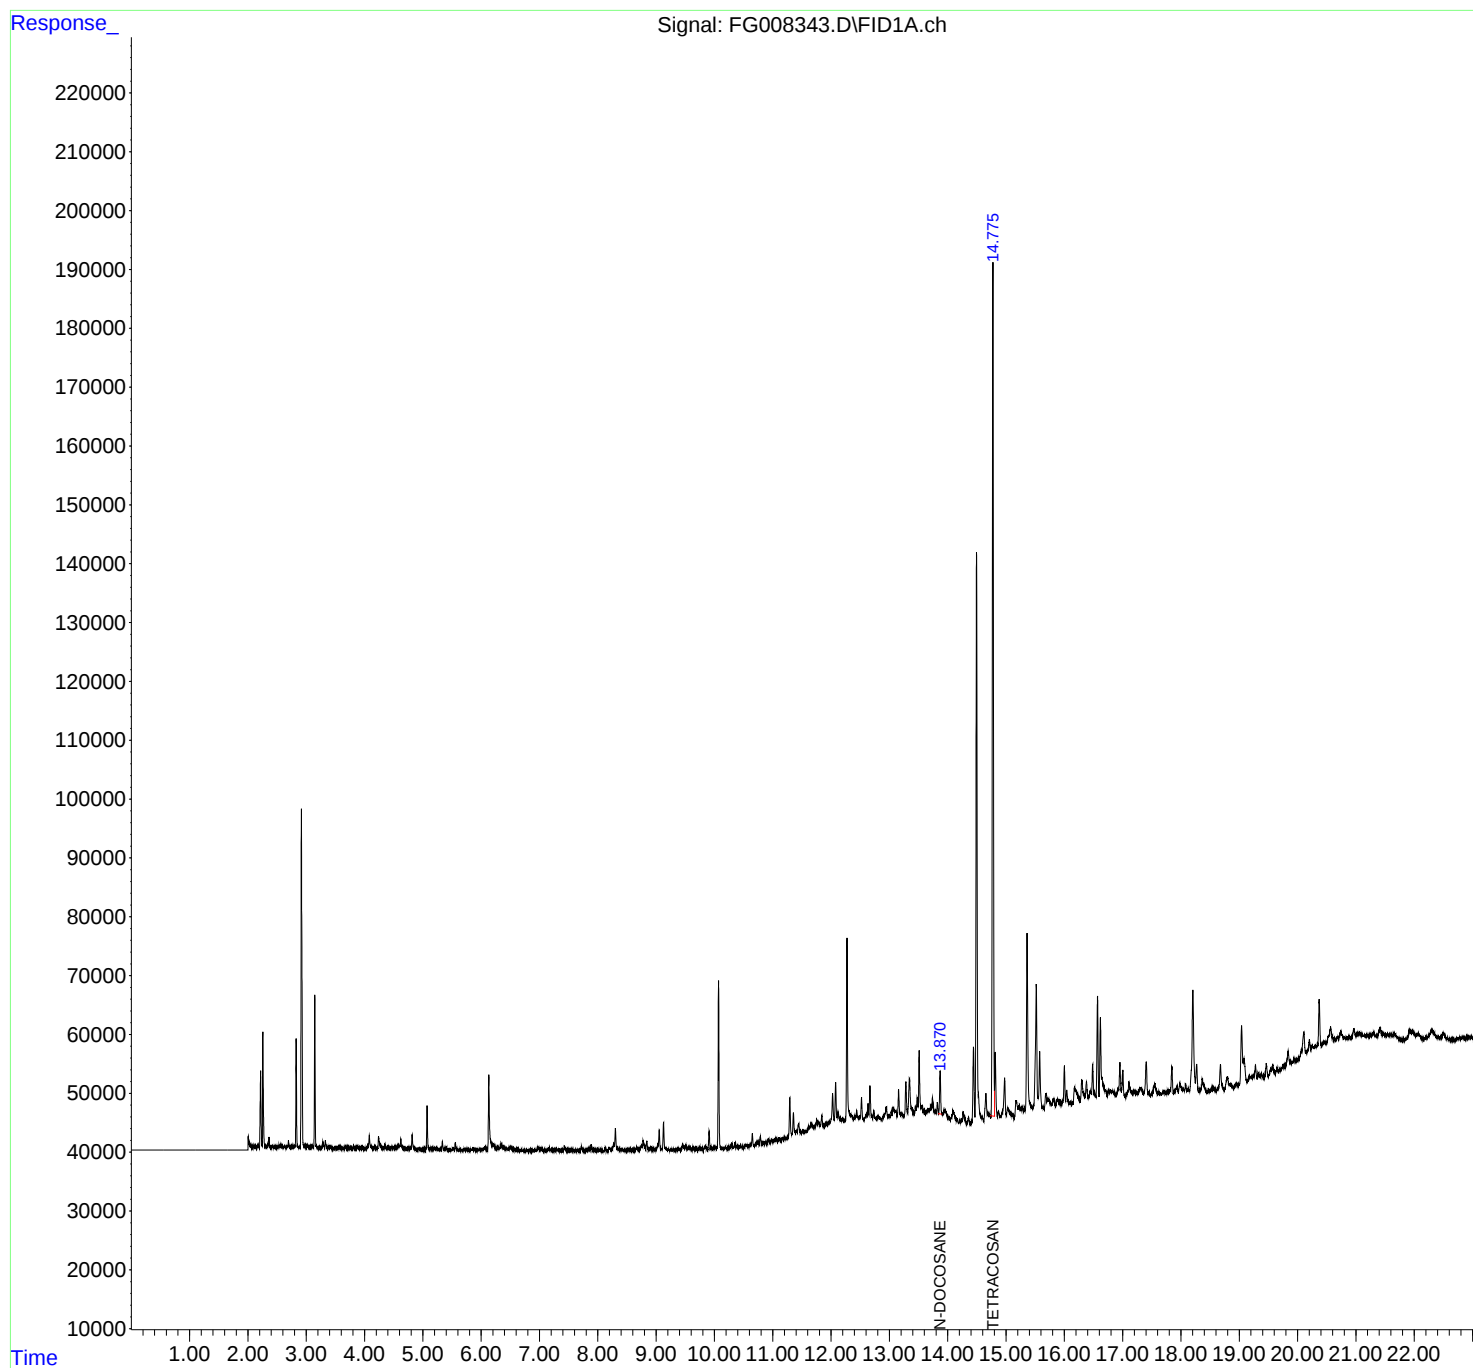


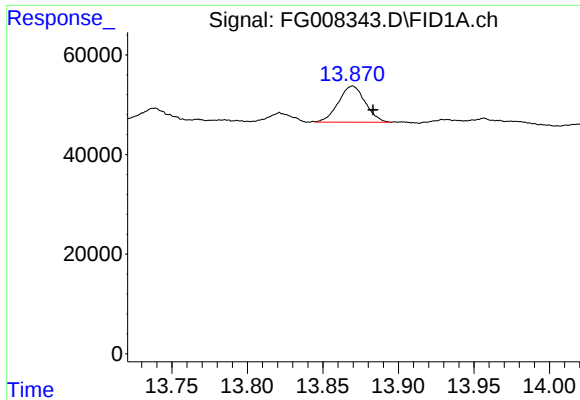

#8 N-DOCOSANE

R.T.: 13.870 min
Delta R.T.: -0.014 min
Response: 90108
Conc: 0.66 ug/ml

Instrument :
FID_G
ClientSampleId :

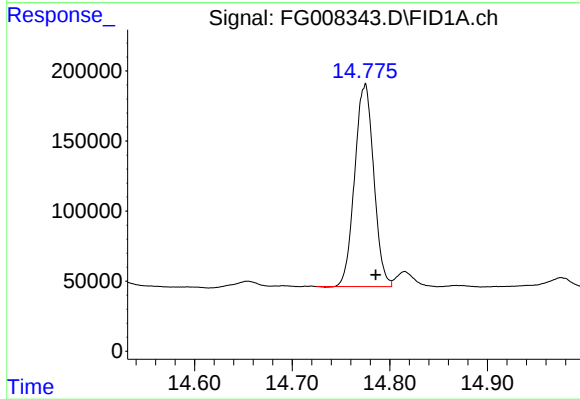

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.775 min
Delta R.T.: -0.011 min
Response: 1959074
Conc: 16.51 ug/ml