

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061622\
Data File : FG009892.D
Signal(s) : FID1A.ch
Acq On : 16 Jun 2022 12:10
Operator : AJ\MA
Sample : N3334-23 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WC-14A-1A-5-GR

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/17/2022
Supervised By :Ankita Jodhani 06/17/2022

Integration File: Sample.e
Quant Time: Jun 17 01:22:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.840	24709	0.235 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061622\
Data File : FG009892.D
Signal(s) : FID1A.ch
Acq On : 16 Jun 2022 12:10
Operator : AJ\MA
Sample : N3334-23 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
WC-14A-1A-5-GR


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/17/2022
Supervised By :Ankita Jodhani 06/17/2022

Integration File: Sample.e
Quant Time: Jun 17 01:22:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

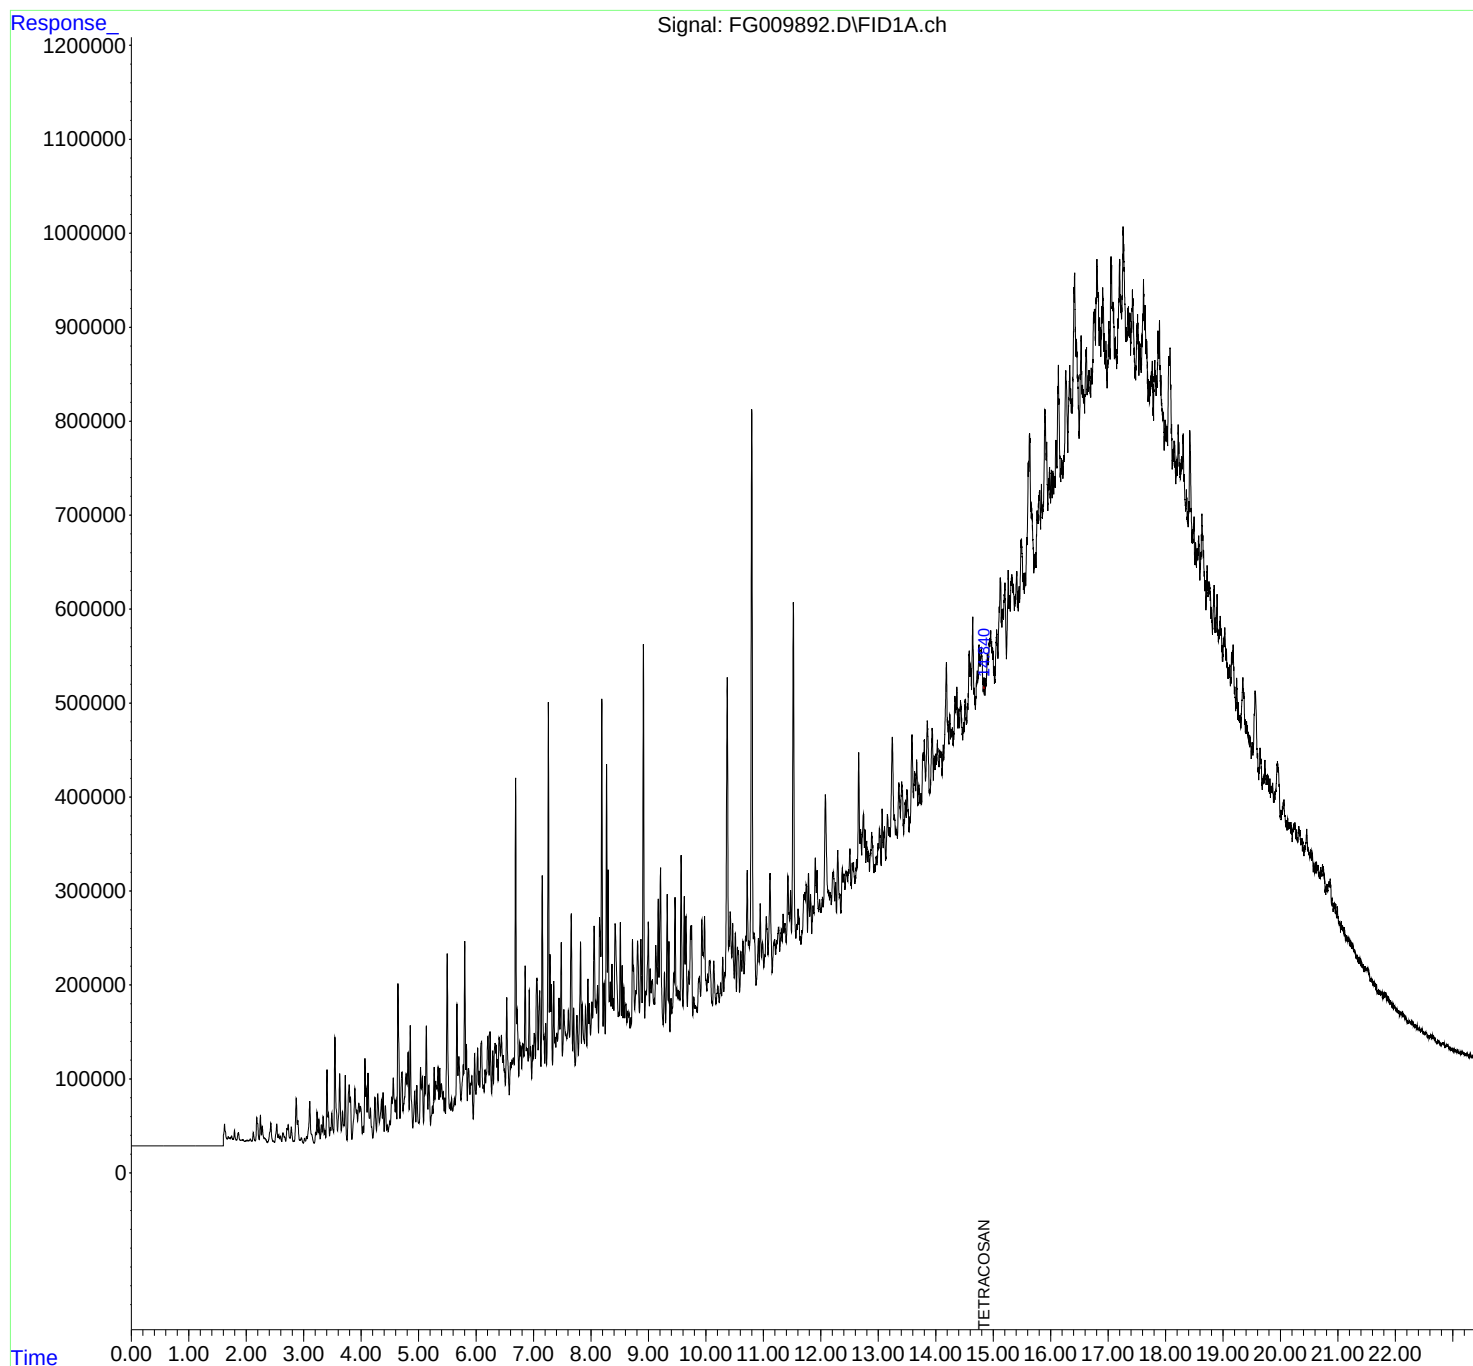

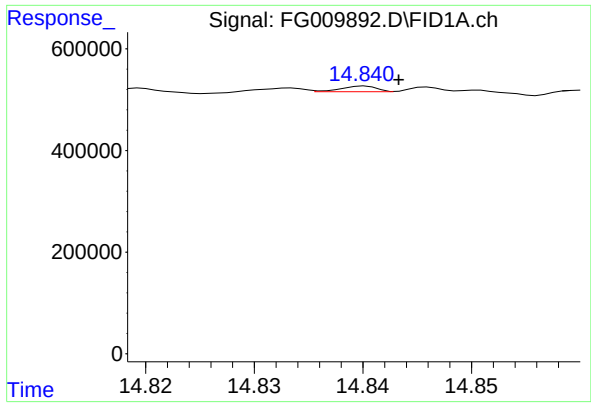

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.840 min
Delta R.T.: -0.003 min
Response: 24709
Conc: 0.23 ug/ml

Instrument :
FID_G
ClientSampleId :
WC-14A-1A-5-GR

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/17/2022
Supervised By :Ankita Jodhani 06/17/2022