

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061719\  
Data File : FG005138.D  
Signal(s) : FID1A.ch  
Acq On : 17 Jun 2019 08:14  
Operator : DD\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jun 17 14:10:32 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG060719.M  
Quant Title :  
QLast Update : Mon Jun 10 08:32:25 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                   | R.T.   | Response | Conc Units  |
|-----------------------------|-------------------|--------|----------|-------------|
| -----                       |                   |        |          |             |
| System Monitoring Compounds |                   |        |          |             |
| Target Compounds            |                   |        |          |             |
| 13)                         | N-TRIACONTANE     | 17.835 | 25219    | 0.180 ug/ml |
| 14)                         | N-DOTRIACONTANE   | 18.682 | 157096   | 1.168 ug/ml |
| 16)                         | N-HEXATRIACONTANE | 20.233 | 290419   | 2.438 ug/ml |
| 18)                         | N-TETRACONTANE    | 21.946 | 347629   | 3.327 ug/ml |
| -----                       |                   |        |          |             |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061719\  
Data File : FG005138.D  
Signal(s) : FID1A.ch  
Acq On : 17 Jun 2019 08:14  
Operator : DD\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jun 17 14:10:32 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG060719.M  
Quant Title :  
QLast Update : Mon Jun 10 08:32:25 2019  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

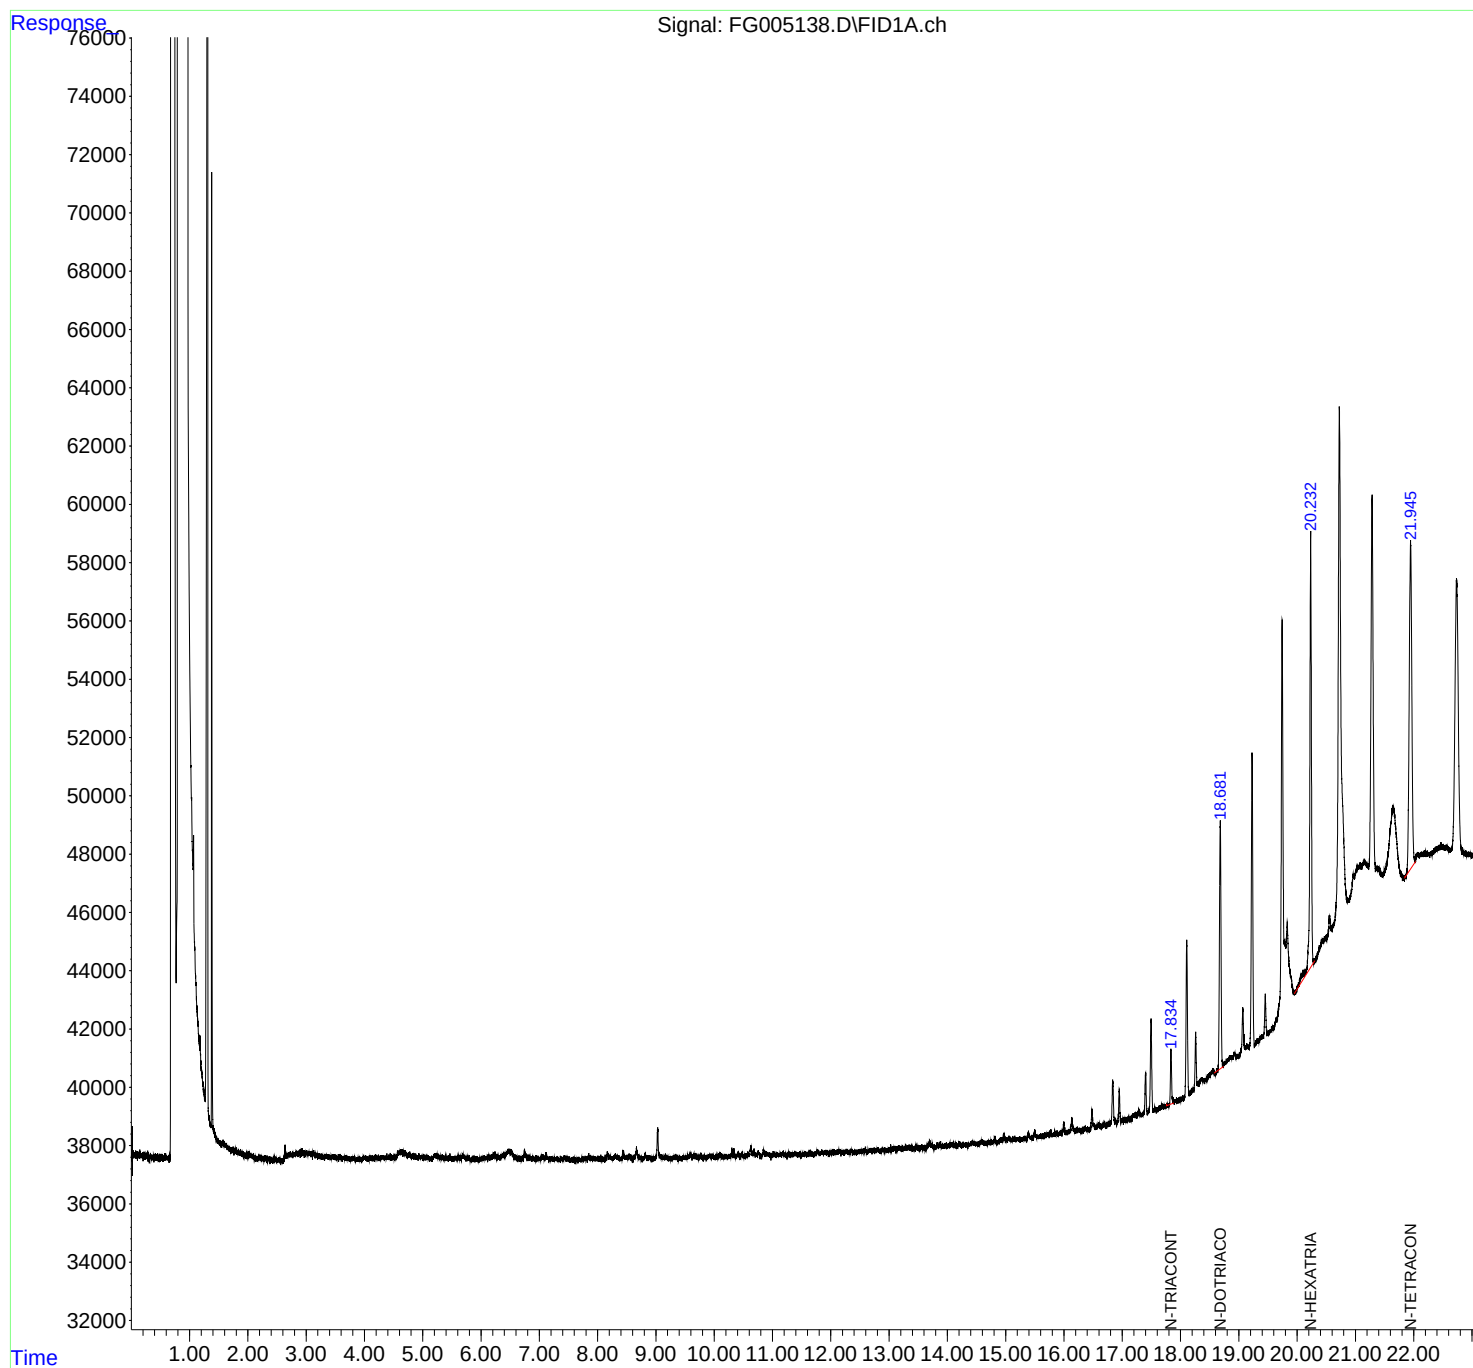

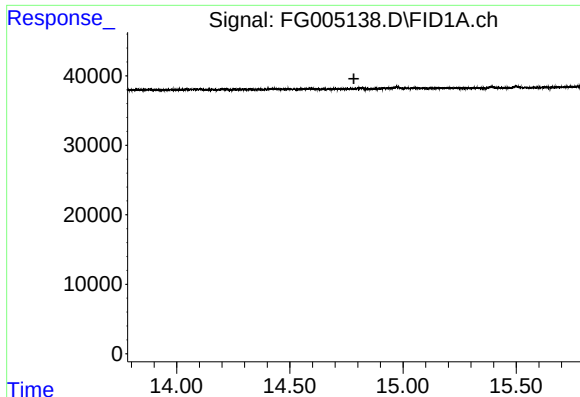


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.783 min  
Response: 0  
Conc: N.D.

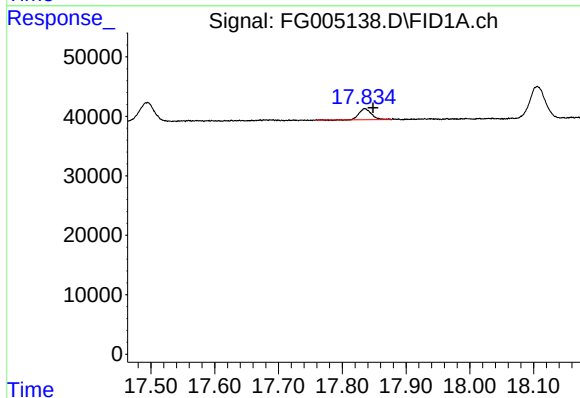


#13 N-TRIACONTANE

R.T.: 17.835 min  
Delta R.T.: -0.013 min  
Response: 25219  
Conc: 0.18 ug/ml

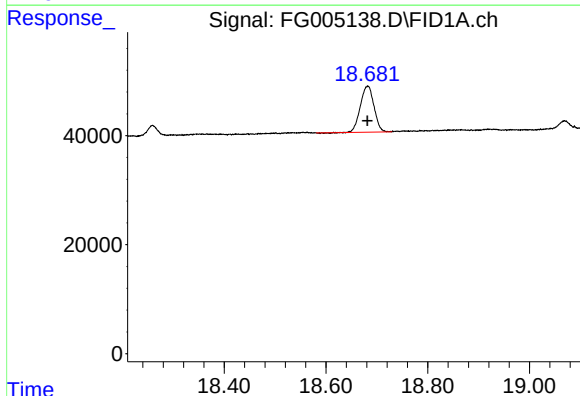


#14 N-DOTRIACONTANE

R.T.: 18.682 min  
Delta R.T.: 0.000 min  
Response: 157096  
Conc: 1.17 ug/ml

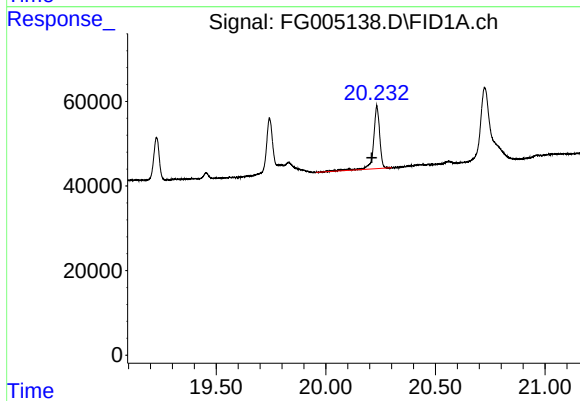

#16 N-HEXATRIACONTANE

R.T.: 20.233 min  
Delta R.T.: 0.023 min  
Response: 290419  
Conc: 2.44 ug/ml

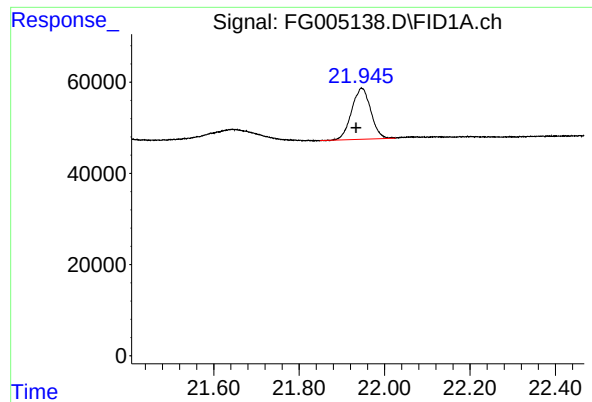

#18 N-TETRACONTANE

R.T.: 21.946 min  
Delta R.T.: 0.013 min  
Response: 347629  
Conc: 3.33 ug/ml