

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061722\
 Data File : FG009907.D
 Signal(s) : FID1A.ch
 Acq On : 17 Jun 2022 20:15
 Operator : AJ\MA
 Sample : N3383-06 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 17 23:49:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
 Quant Title :
 QLast Update : Wed Jun 01 13:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.835	235405	2.237 ug/ml
Target Compounds			
7) N-EICOSANE	12.758	1924987	15.740 ug/ml
8) N-DOCOSANE	13.929	247927	2.056 ug/ml
10) N-TETRACOSANE	15.038	289811	2.473 ug/ml
11) N-HEXACOSANE	16.063	241897	2.132 ug/ml
12) N-OCTACOSANE	17.016	181335	1.585 ug/ml
13) N-TRIACONTANE	17.908	232668	2.161 ug/ml
14) N-DOTRIACONTANE	18.740	136388	1.296 ug/ml
15) N-TETRATRIACONTANE	19.530	182876	1.905 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061722\
Data File : FG009907.D
Signal(s) : FID1A.ch
Acq On : 17 Jun 2022 20:15
Operator : AJ\MA
Sample : N3383-06 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 23:49:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

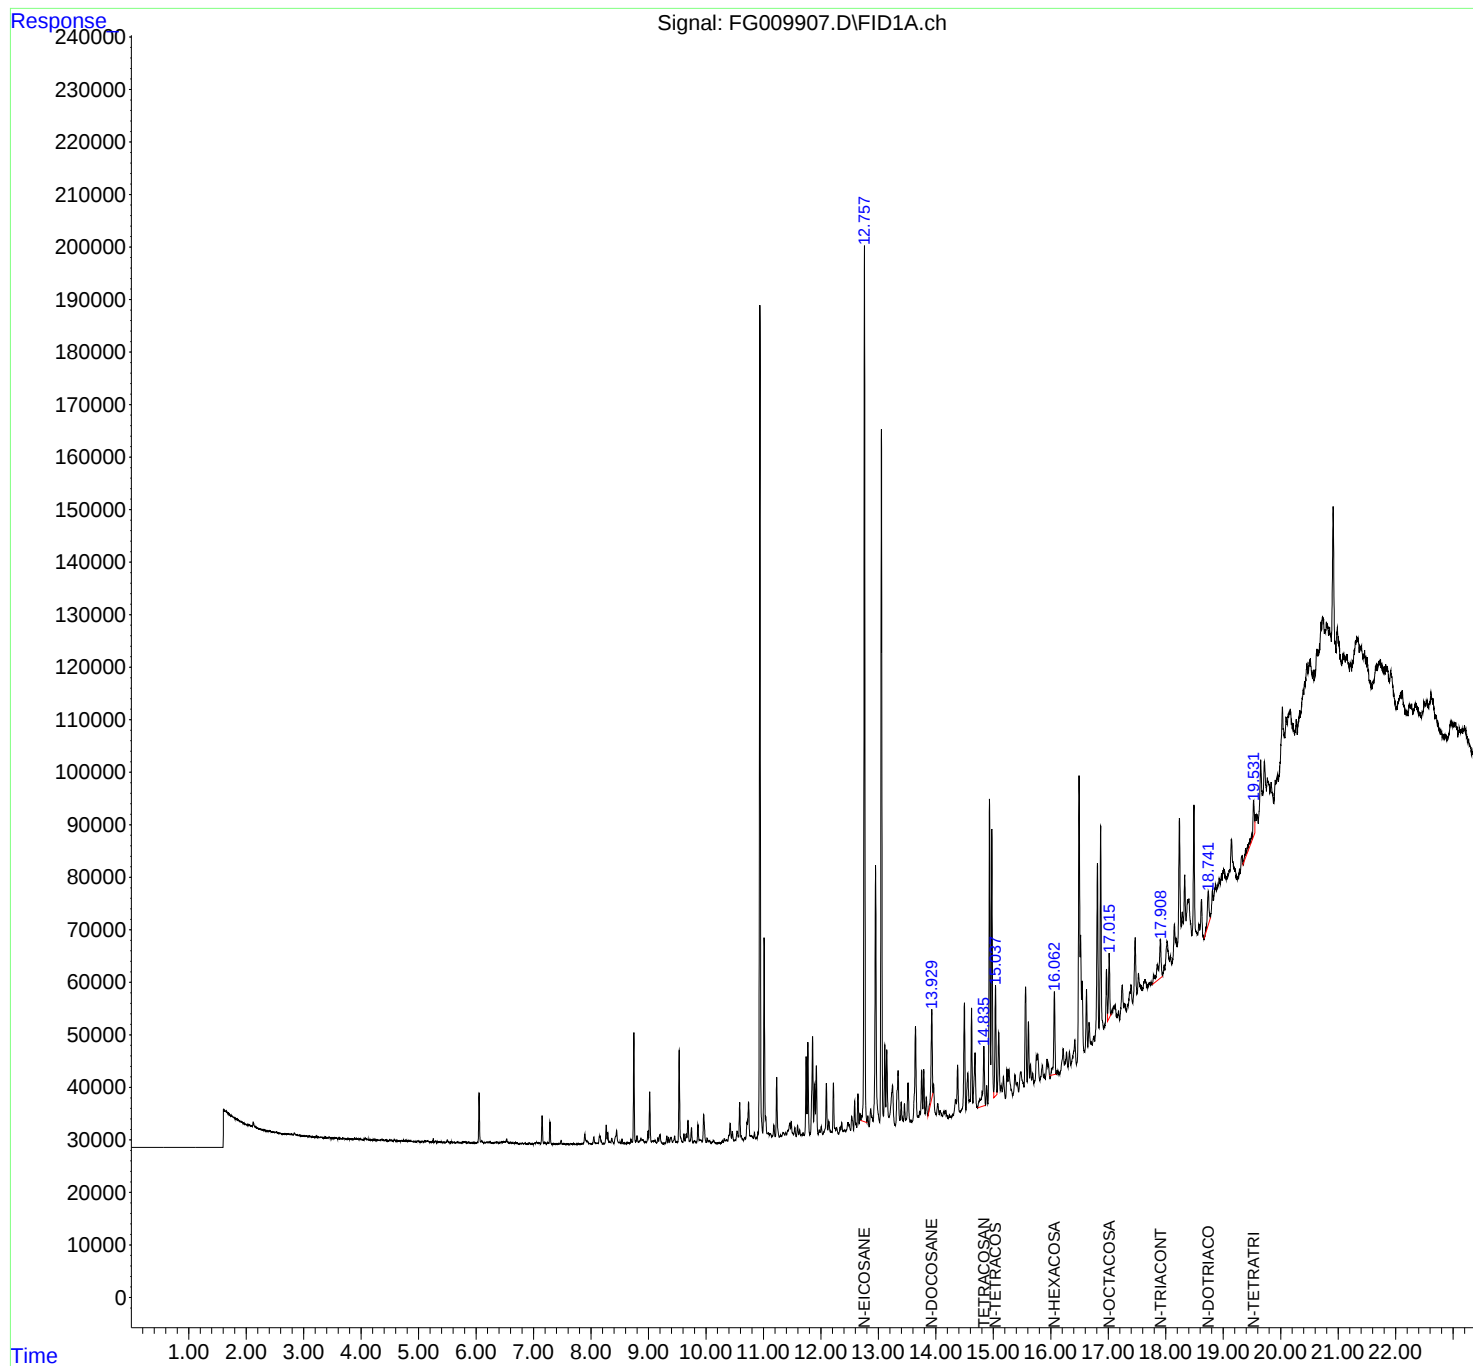


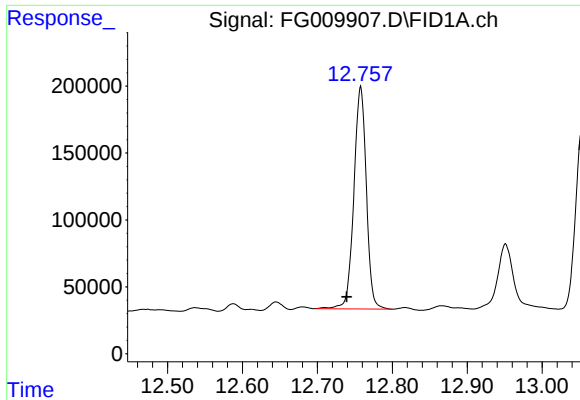

#7 N-EICOSANE


R.T.: 12.758 min
Delta R.T.: 0.019 min
Response: 1924987
Conc: 15.74 ug/ml

Instrument :
FID_G
ClientSampleId :

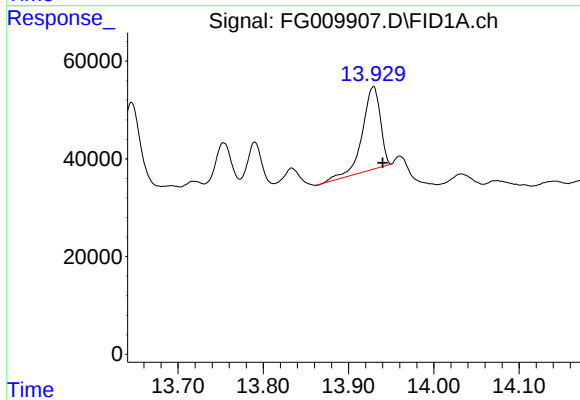


#8 N-DOCOSANE

R.T.: 13.929 min
Delta R.T.: -0.011 min
Response: 247927
Conc: 2.06 ug/ml

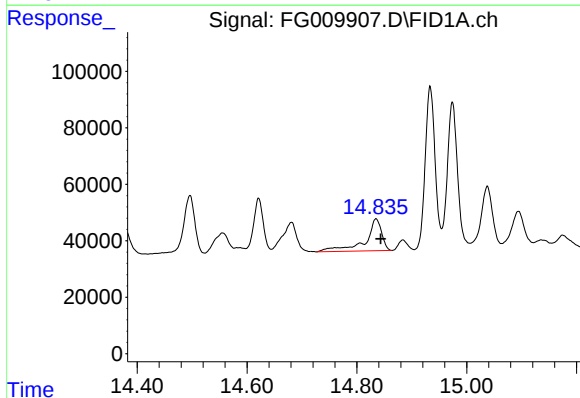


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.835 min
Delta R.T.: -0.008 min
Response: 235405
Conc: 2.24 ug/ml

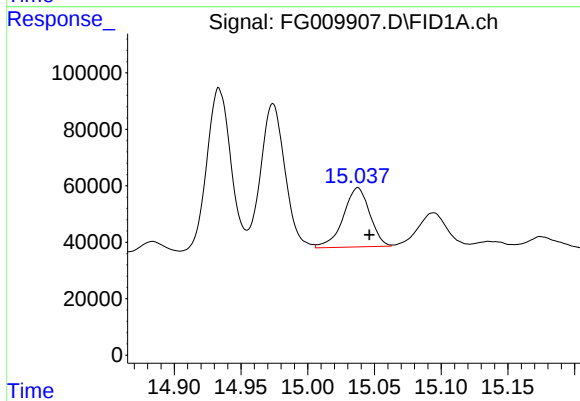

#10 N-TETRACOSANE


R.T.: 15.038 min
Delta R.T.: -0.009 min
Response: 289811
Conc: 2.47 ug/ml

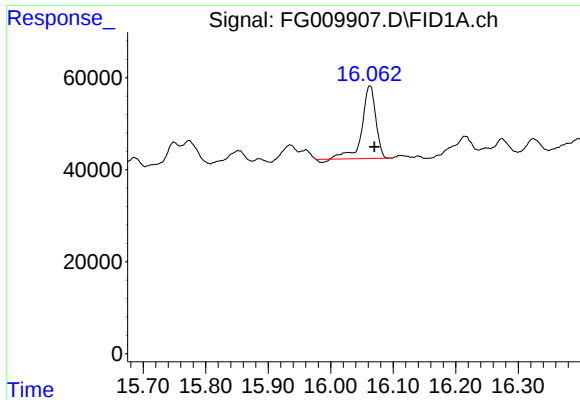

#11 N-HEXACOSANE


R.T.: 16.063 min
Delta R.T.: -0.007 min
Response: 241897
Conc: 2.13 ug/ml

Instrument :
FID_G
ClientSampleId :

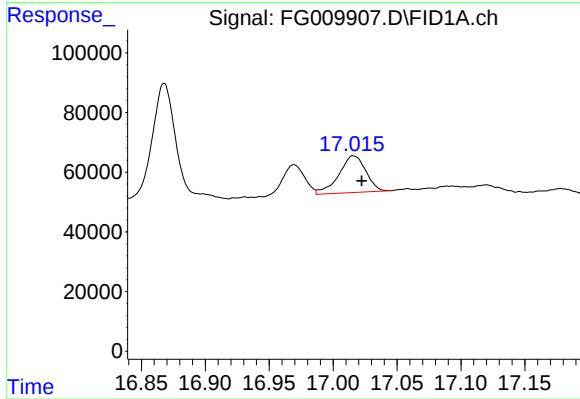


#12 N-OCTACOSANE

R.T.: 17.016 min
Delta R.T.: -0.007 min
Response: 181335
Conc: 1.58 ug/ml

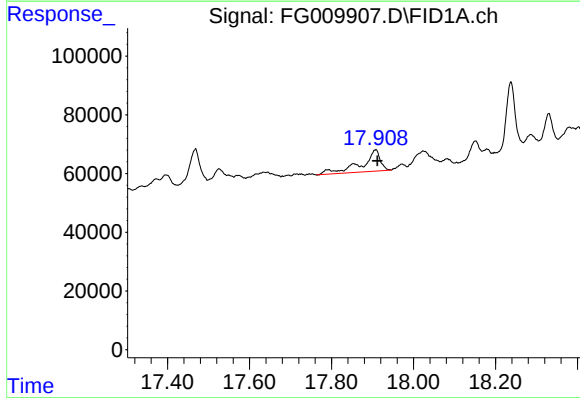


#13 N-TRIACONTANE

R.T.: 17.908 min
Delta R.T.: -0.004 min
Response: 232668
Conc: 2.16 ug/ml

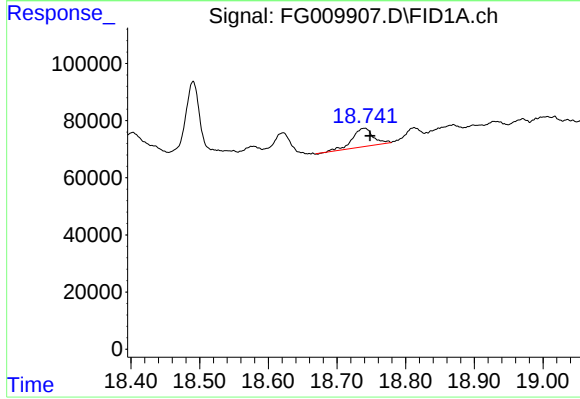

#14 N-DOTRIACONTANE

R.T.: 18.740 min
Delta R.T.: -0.008 min
Response: 136388
Conc: 1.30 ug/ml

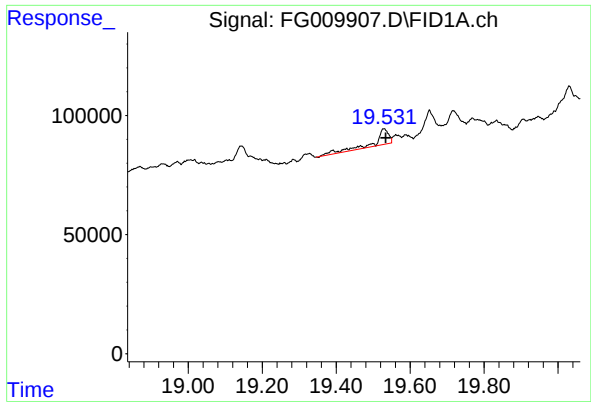

#15 N-TETRATRIACONTANE

R.T.: 19.530 min
Delta R.T.: -0.005 min
Response: 182876
Conc: 1.90 ug/ml

Instrument :
FID_G
ClientSampleId :