

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061722\
 Data File : FG009908.D
 Signal(s) : FID1A.ch
 Acq On : 17 Jun 2022 20:44
 Operator : AJ\MA
 Sample : N3383-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 17 23:50:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
 Quant Title :
 QLast Update : Wed Jun 01 13:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.835	195431	1.857 ug/ml
Target Compounds			
6) N-OCTADECANE	11.461	61016	0.483 ug/ml
7) N-EICOSANE	12.757	926304	7.574 ug/ml
8) N-DOCOSANE	13.921	128717	1.067 ug/ml
10) N-TETRACOSANE	15.092	118363	1.010 ug/ml
15) N-TETRATRIACONTANE	19.526	105186	1.096 ug/ml
16) N-HEXATRIACONTANE	20.338f	199356	2.467 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061722\
Data File : FG009908.D
Signal(s) : FID1A.ch
Acq On : 17 Jun 2022 20:44
Operator : AJ\MA
Sample : N3383-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 23:50:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

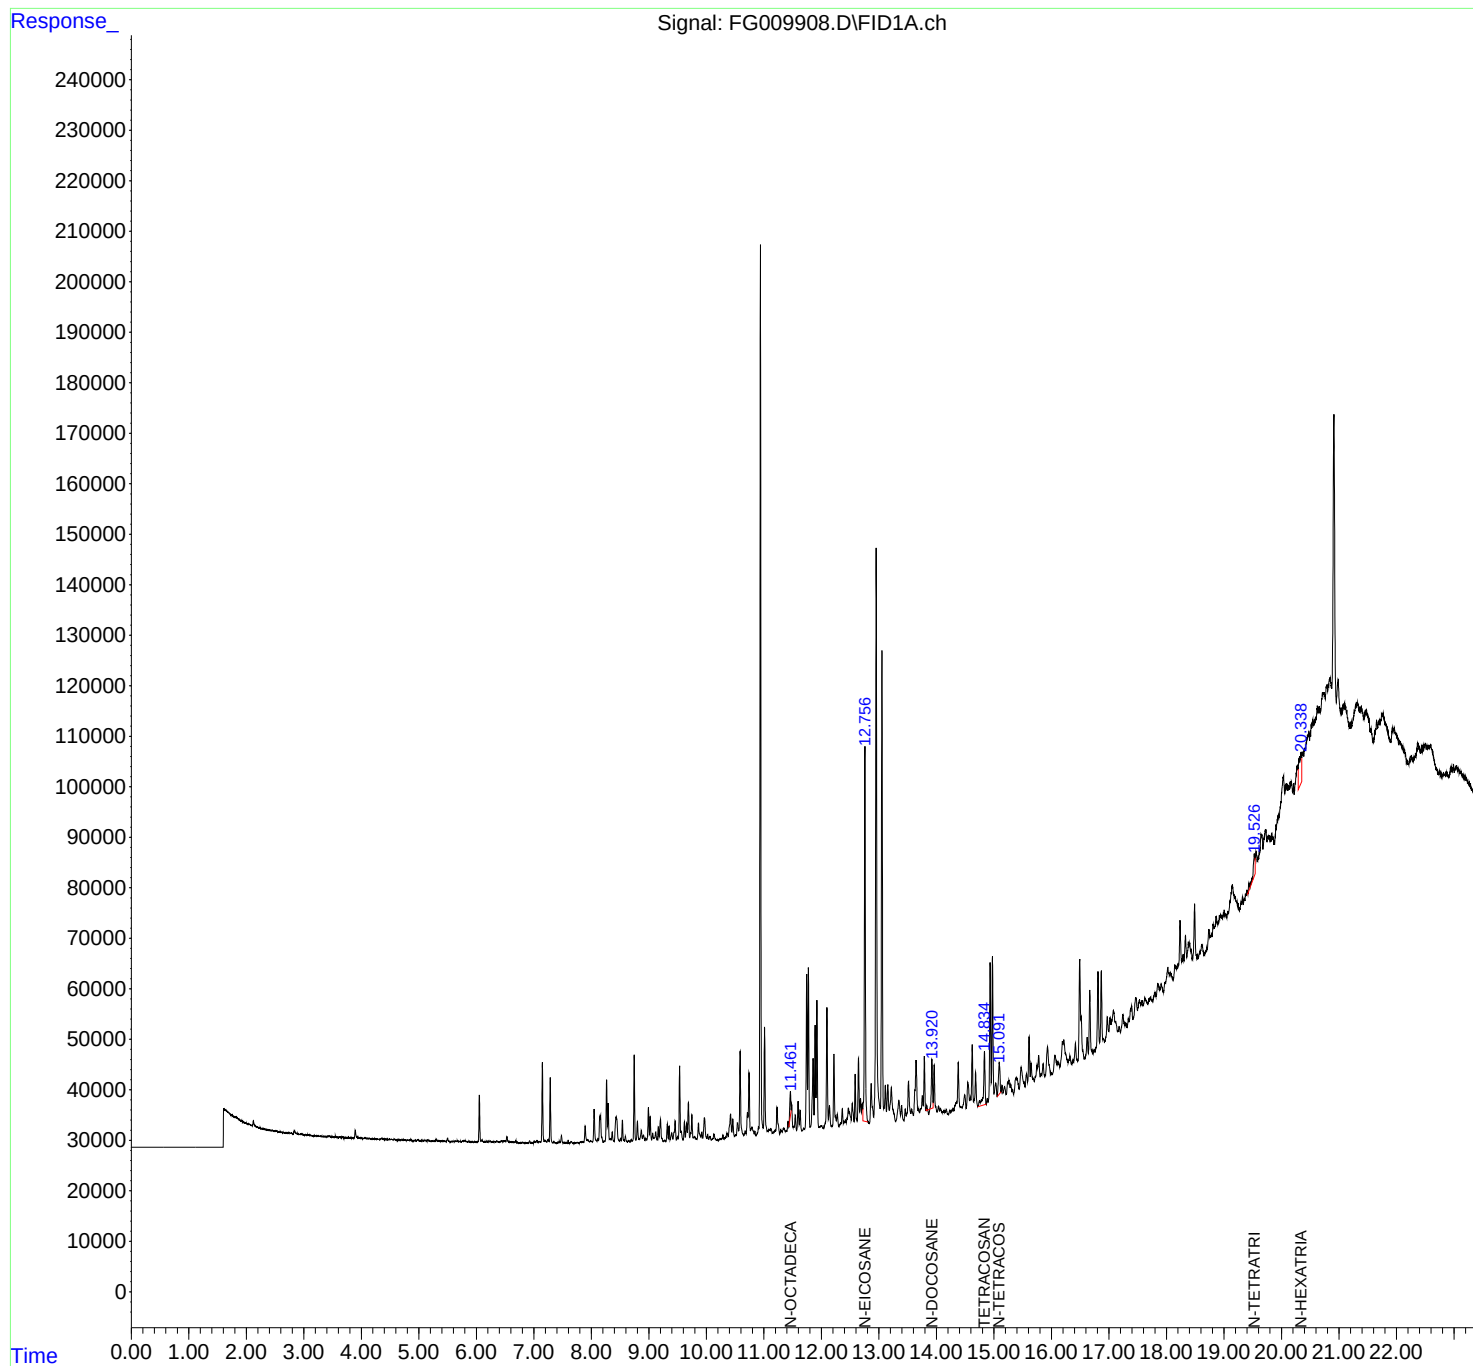


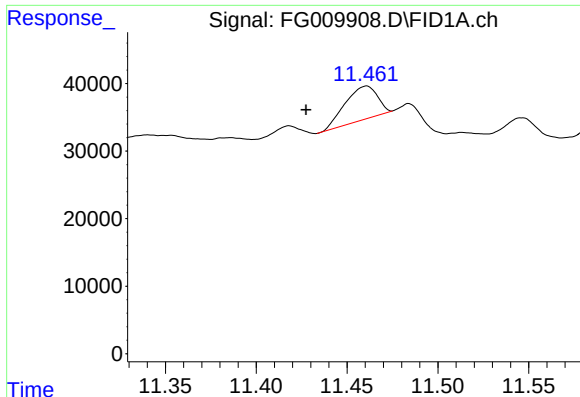

#6 N-OCTADECANE


R.T.: 11.461 min
Delta R.T.: 0.033 min
Response: 61016
Conc: 0.48 ug/ml

Instrument :
FID_G
ClientSampleId :

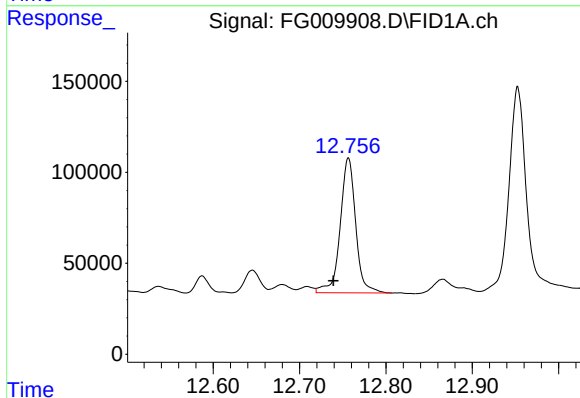


#7 N-EICOSANE

R.T.: 12.757 min
Delta R.T.: 0.017 min
Response: 926304
Conc: 7.57 ug/ml

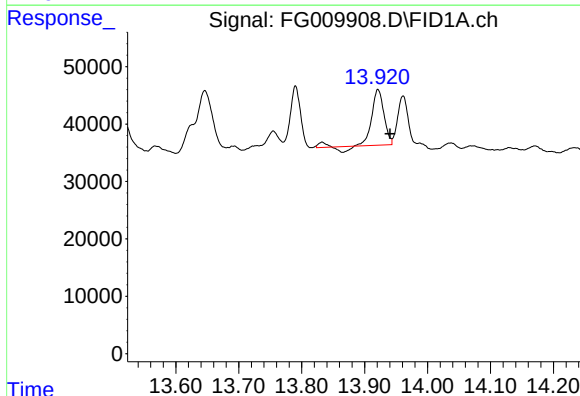


#8 N-DOCOSANE

R.T.: 13.921 min
Delta R.T.: -0.019 min
Response: 128717
Conc: 1.07 ug/ml

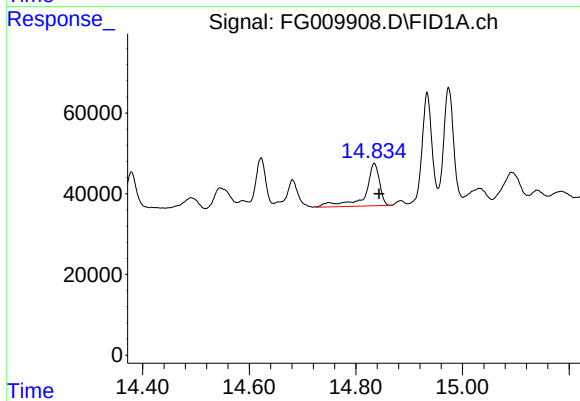

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.835 min
Delta R.T.: -0.009 min
Response: 195431
Conc: 1.86 ug/ml

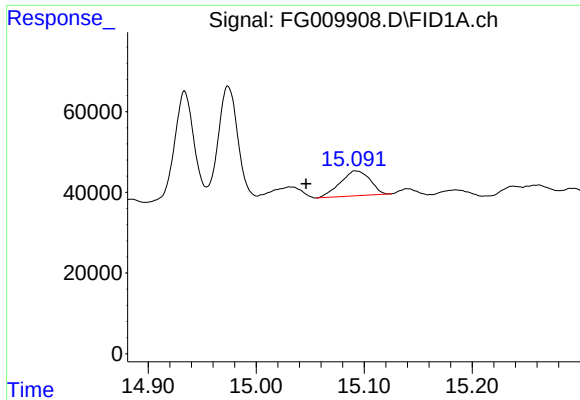

#10 N-TETRACOSANE


R.T.: 15.092 min
Delta R.T.: 0.046 min
Response: 118363
Conc: 1.01 ug/ml

Instrument :
FID_G
ClientSampleId :

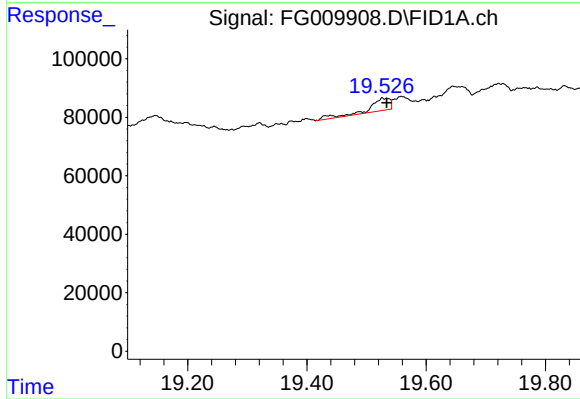

#15 N-TETRATRIACONTANE

R.T.: 19.526 min
Delta R.T.: -0.008 min
Response: 105186
Conc: 1.10 ug/ml

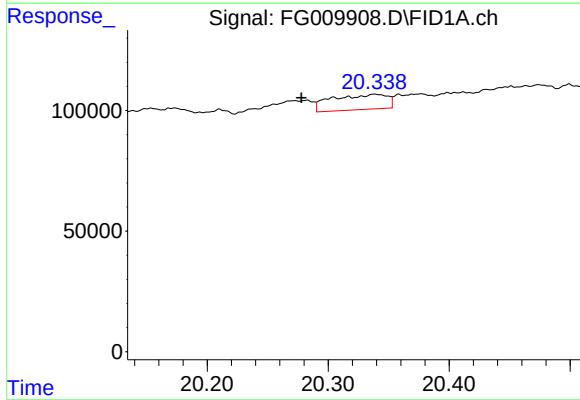

#16 N-HEXATRIACONTANE

R.T.: 20.338 min
Delta R.T.: 0.060 min
Response: 199356
Conc: 2.47 ug/ml