

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061722\
Data File : FG009909.D
Signal(s) : FID1A.ch
Acq On : 17 Jun 2022 21:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 23:50:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.835	1810771	17.203 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.905	183499	1.704 ug/ml
14) N-DOTRIACONTANE	18.741	229291	2.178 ug/ml
15) N-TETRATRIACONTANE	19.527	198389	2.066 ug/ml
16) N-HEXATRIACONTANE	20.267	121473	1.503 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061722\
Data File : FG009909.D
Signal(s) : FID1A.ch
Acq On : 17 Jun 2022 21:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 23:50:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

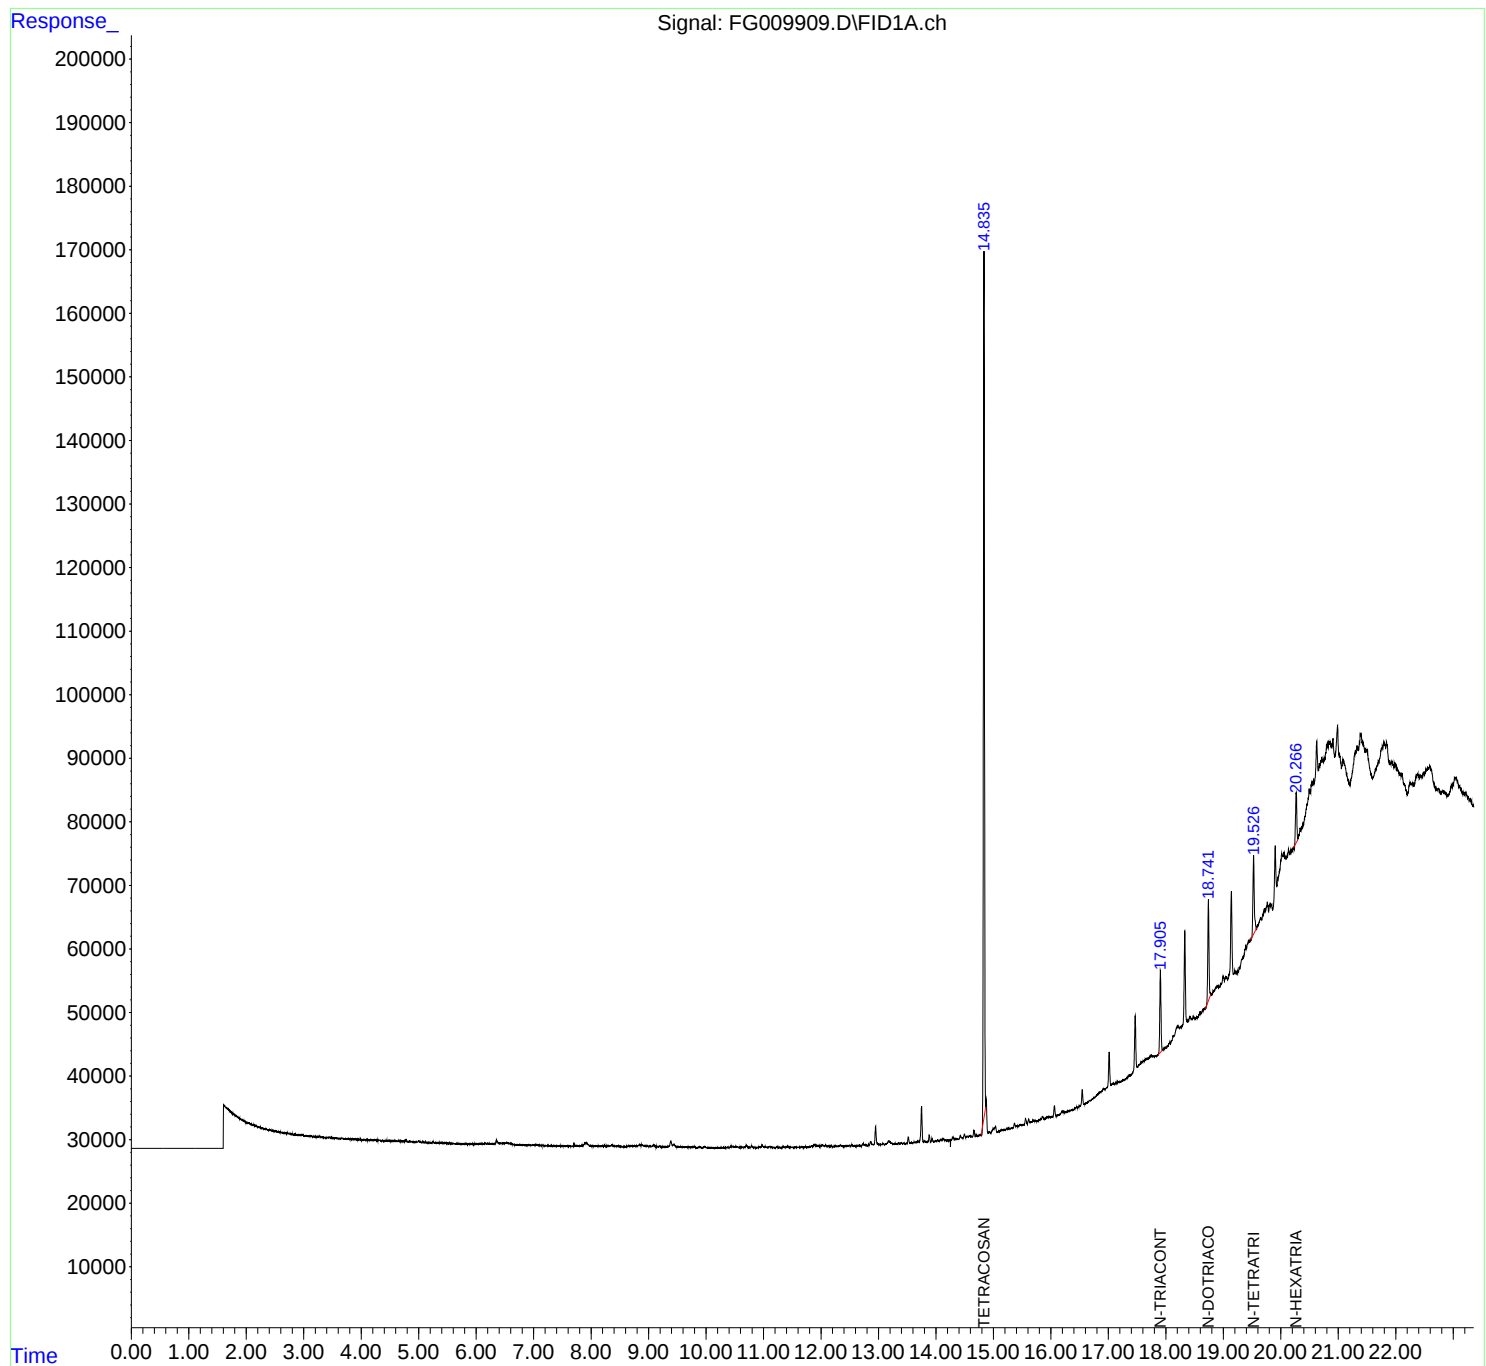


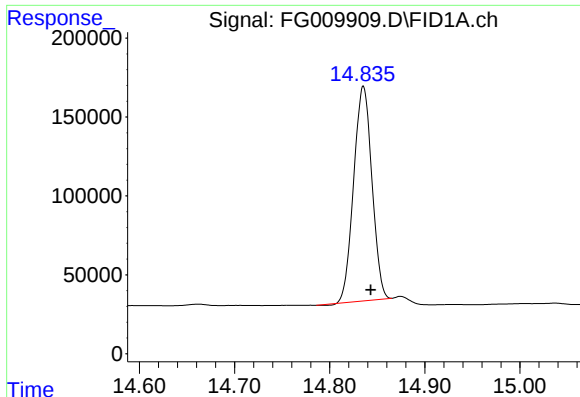

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.835 min
Delta R.T.: -0.008 min
Response: 1810771
Conc: 17.20 ug/ml

Instrument :
FID_G
ClientSampleId :

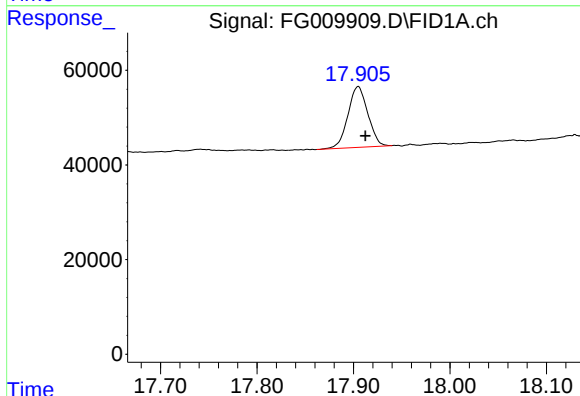


#13 N-TRIACONTANE

R.T.: 17.905 min
Delta R.T.: -0.007 min
Response: 183499
Conc: 1.70 ug/ml

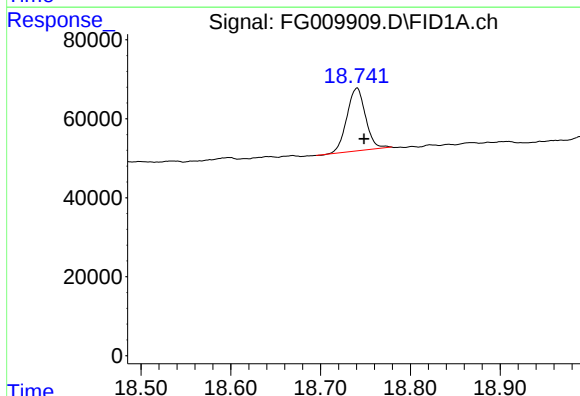


#14 N-DOTRIACONTANE

R.T.: 18.741 min
Delta R.T.: -0.008 min
Response: 229291
Conc: 2.18 ug/ml

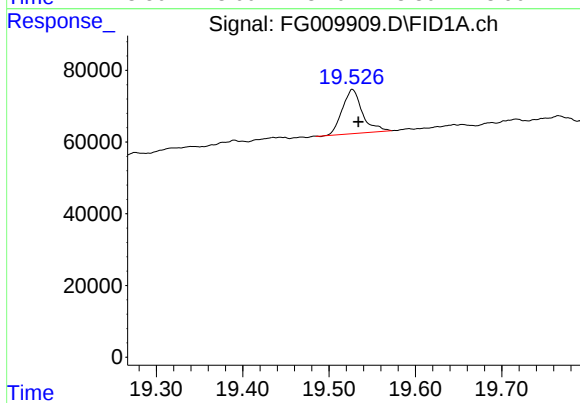

#15 N-TETRATRIACONTANE

R.T.: 19.527 min
Delta R.T.: -0.007 min
Response: 198389
Conc: 2.07 ug/ml

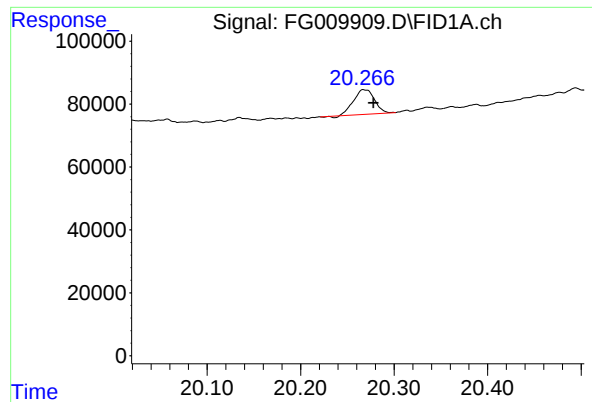

#16 N-HEXATRIACONTANE

R.T.: 20.267 min
Delta R.T.: -0.011 min
Response: 121473
Conc: 1.50 ug/ml

Instrument :

FID_G

ClientSampleId :