

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061722\  
Data File : FG009900.D  
Signal(s) : FID1A.ch  
Acq On : 17 Jun 2022 16:48  
Operator : AJ\MA  
Sample : N3334-23 10X  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
WC-14A-1A-5-GR

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/20/2022  
Supervised By :Ankita Jodhani 06/20/2022

Integration File: Sample.e  
Quant Time: Jun 18 00:06:28 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG060122.M  
Quant Title :  
QLast Update : Wed Jun 01 13:06:30 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.840 | 11194    | 0.106 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061722\  
Data File : FG009900.D  
Signal(s) : FID1A.ch  
Acq On : 17 Jun 2022 16:48  
Operator : AJ\MA  
Sample : N3334-23 10X  
Misc :  
ALS Vial : 5 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
WC-14A-1A-5-GR


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/20/2022  
Supervised By :Ankita Jodhani 06/20/2022

Integration File: Sample.e  
Quant Time: Jun 18 00:06:28 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG060122.M  
Quant Title :  
QLast Update : Wed Jun 01 13:06:30 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

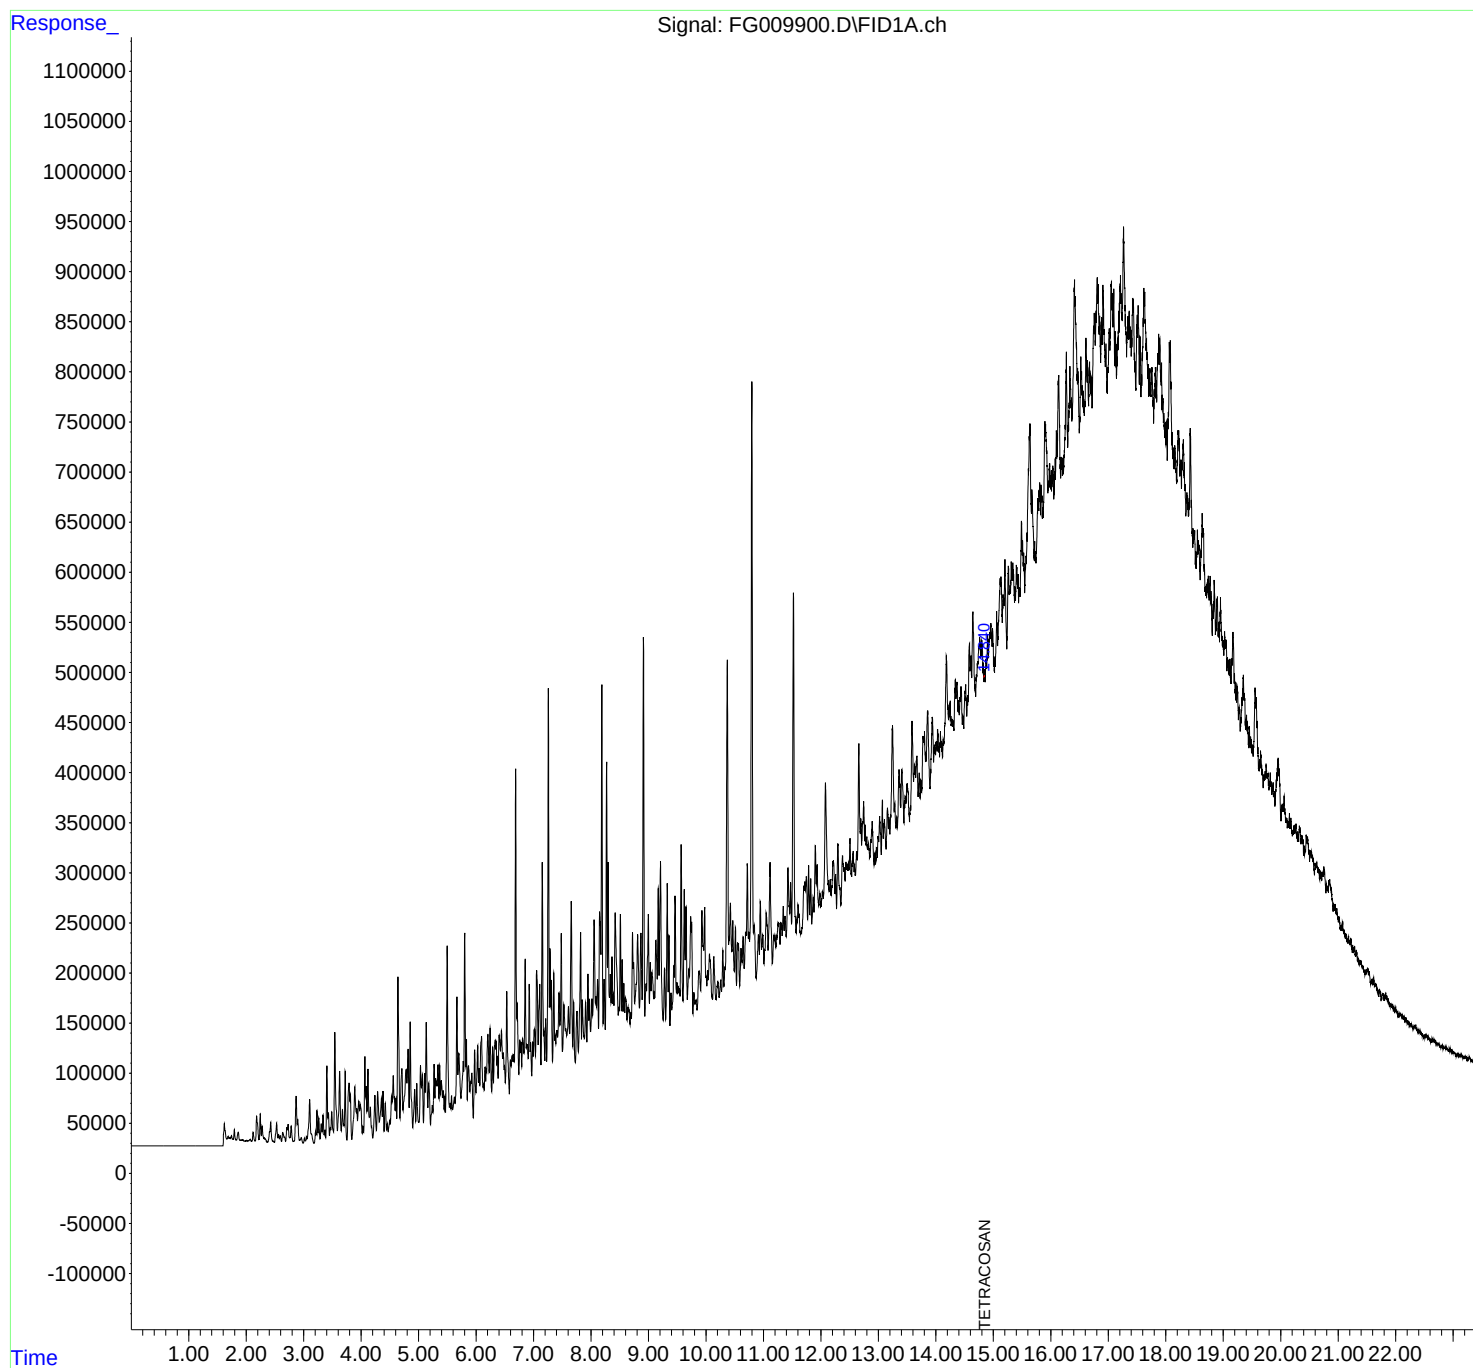

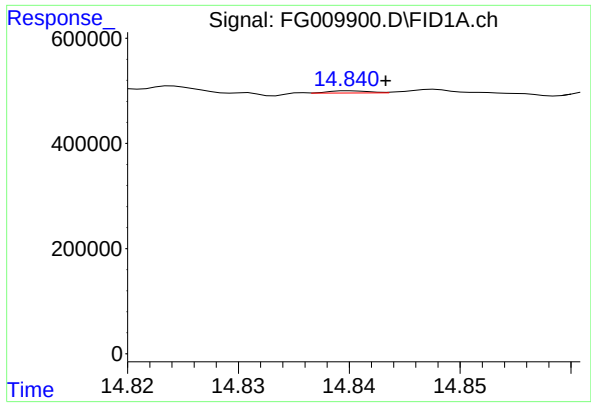

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.840 min  
Delta R.T.: -0.004 min  
Response: 11194  
Conc: 0.11 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
WC-14A-1A-5-GR

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/20/2022  
Supervised By :Ankita Jodhani 06/20/2022