

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061821\
 Data File : FG008359.D
 Signal(s) : FID1A.ch
 Acq On : 18 Jun 2021 13:43
 Operator : DD\AJ
 Sample : PB137199BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 18 23:48:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.772	2107715	17.760 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.960	208698	1.551 ug/ml
13) N-TRIACONTANE	17.843	131501	1.030 ug/ml
14) N-DOTRIACONTANE	18.678	176858	1.423 ug/ml
15) N-TETRATRIACONTANE	19.463	121401	1.038 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061821\
Data File : FG008359.D
Signal(s) : FID1A.ch
Acq On : 18 Jun 2021 13:43
Operator : DD\AJ
Sample : PB137199BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 18 23:48:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

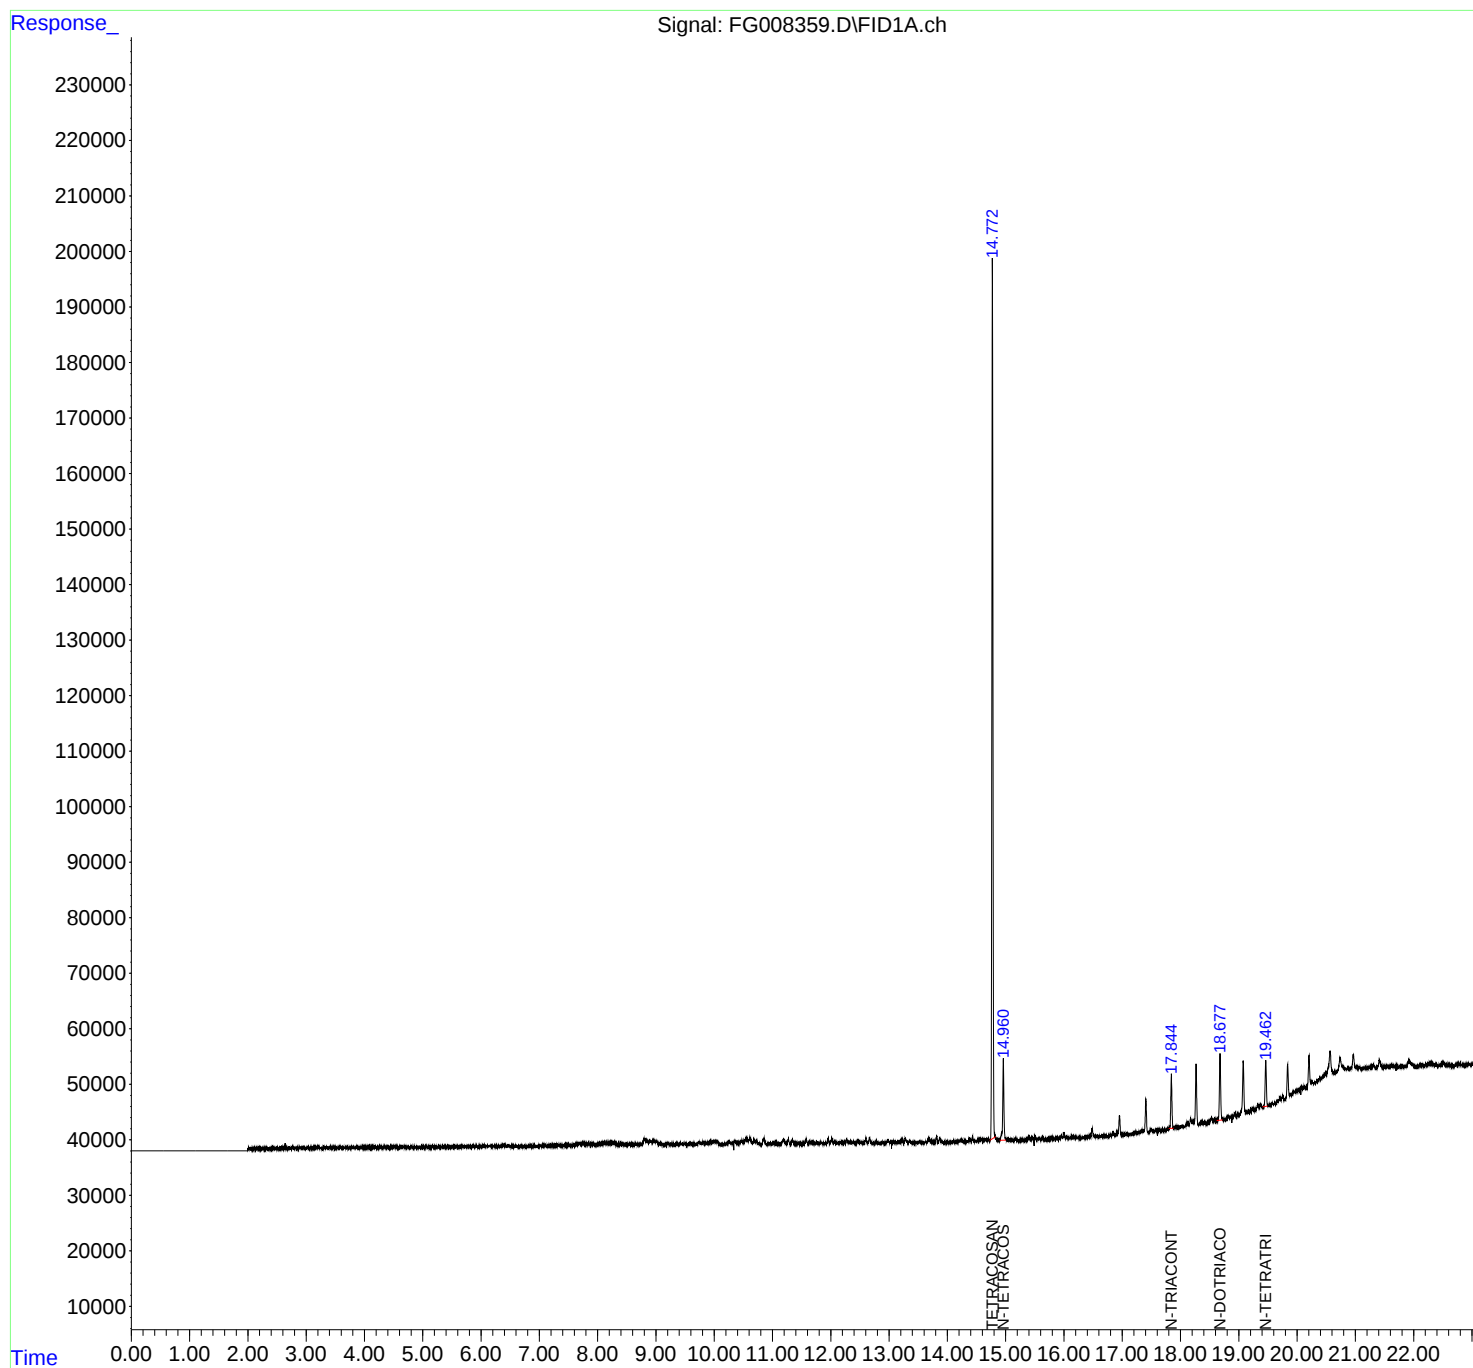


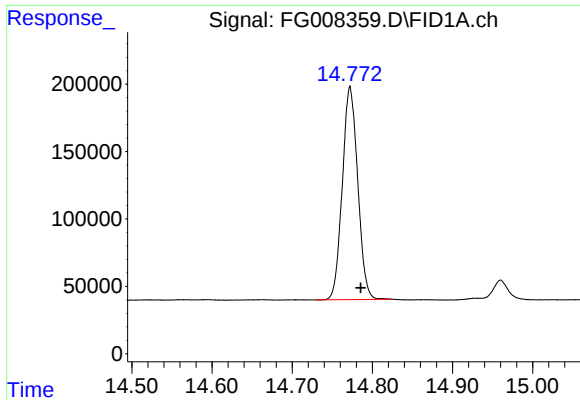

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.772 min
Delta R.T.: -0.013 min
Response: 2107715
Conc: 17.76 ug/ml

Instrument :
FID_G
ClientSampleId :

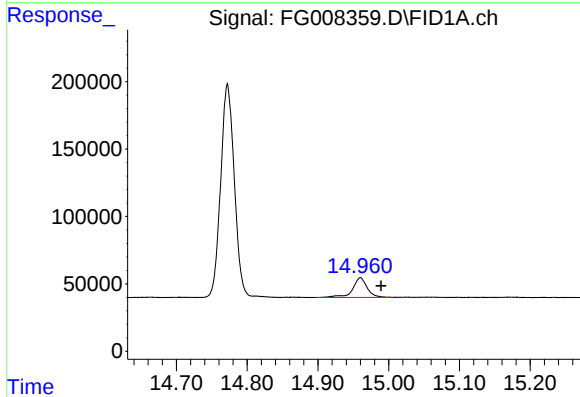


#10 N-TETRACOSANE

R.T.: 14.960 min
Delta R.T.: -0.029 min
Response: 208698
Conc: 1.55 ug/ml

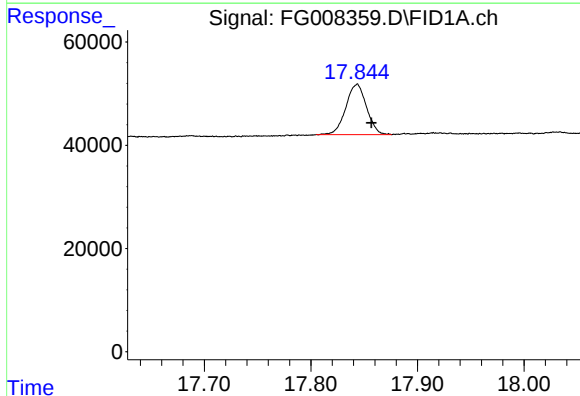


#13 N-TRIACONTANE

R.T.: 17.843 min
Delta R.T.: -0.014 min
Response: 131501
Conc: 1.03 ug/ml

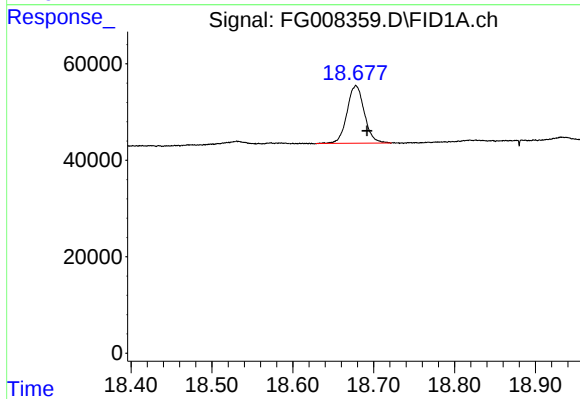

#14 N-DOTRIACONTANE

R.T.: 18.678 min
Delta R.T.: -0.014 min
Response: 176858
Conc: 1.42 ug/ml

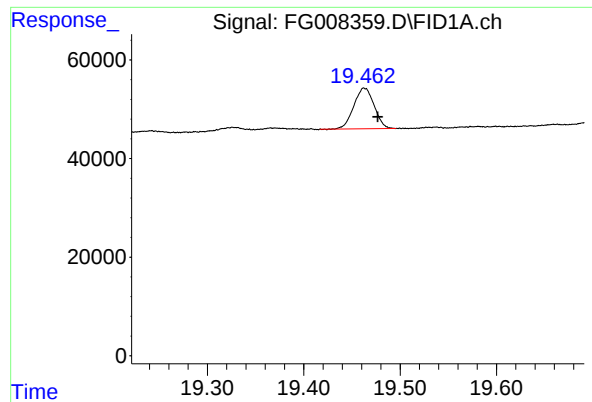

#15 N-TETRATRIACONTANE

R.T.: 19.463 min

Delta R.T.: -0.014 min

Response: 121401

Conc: 1.04 ug/ml

Instrument :
FID_G
ClientSampleId :