

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061821\
 Data File : FG008365.D
 Signal(s) : FID1A.ch
 Acq On : 18 Jun 2021 17:27
 Operator : DD\AJ
 Sample : M2708-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 18 23:49:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.772	1296272	10.923 ug/ml
Target Compounds			
7) N-EICOSANE	12.731	209590	1.531 ug/ml
8) N-DOCOSANE	13.892	180593	1.331 ug/ml
10) N-TETRACOSANE	15.019	57733	0.429 ug/ml
11) N-HEXACOSANE	16.028	540019	4.109 ug/ml
12) N-OCTACOSANE	16.988	2238074	17.267 ug/ml
13) N-TRIACONTANE	17.853	1433139	11.226 ug/ml
14) N-DOTRIACONTANE	18.685	2075264	16.700 ug/ml
15) N-TETRATRIACONTANE	19.490	1779146	15.209 ug/ml
16) N-HEXATRIACONTANE	20.220	2450493	22.126 ug/ml
17) N-OCTATRIACONTANE	20.973	456311	4.417 ug/ml
18) N-TETRACONTANE	21.896	72756	0.678 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061821\
Data File : FG008365.D
Signal(s) : FID1A.ch
Acq On : 18 Jun 2021 17:27
Operator : DD\AJ
Sample : M2708-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 18 23:49:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

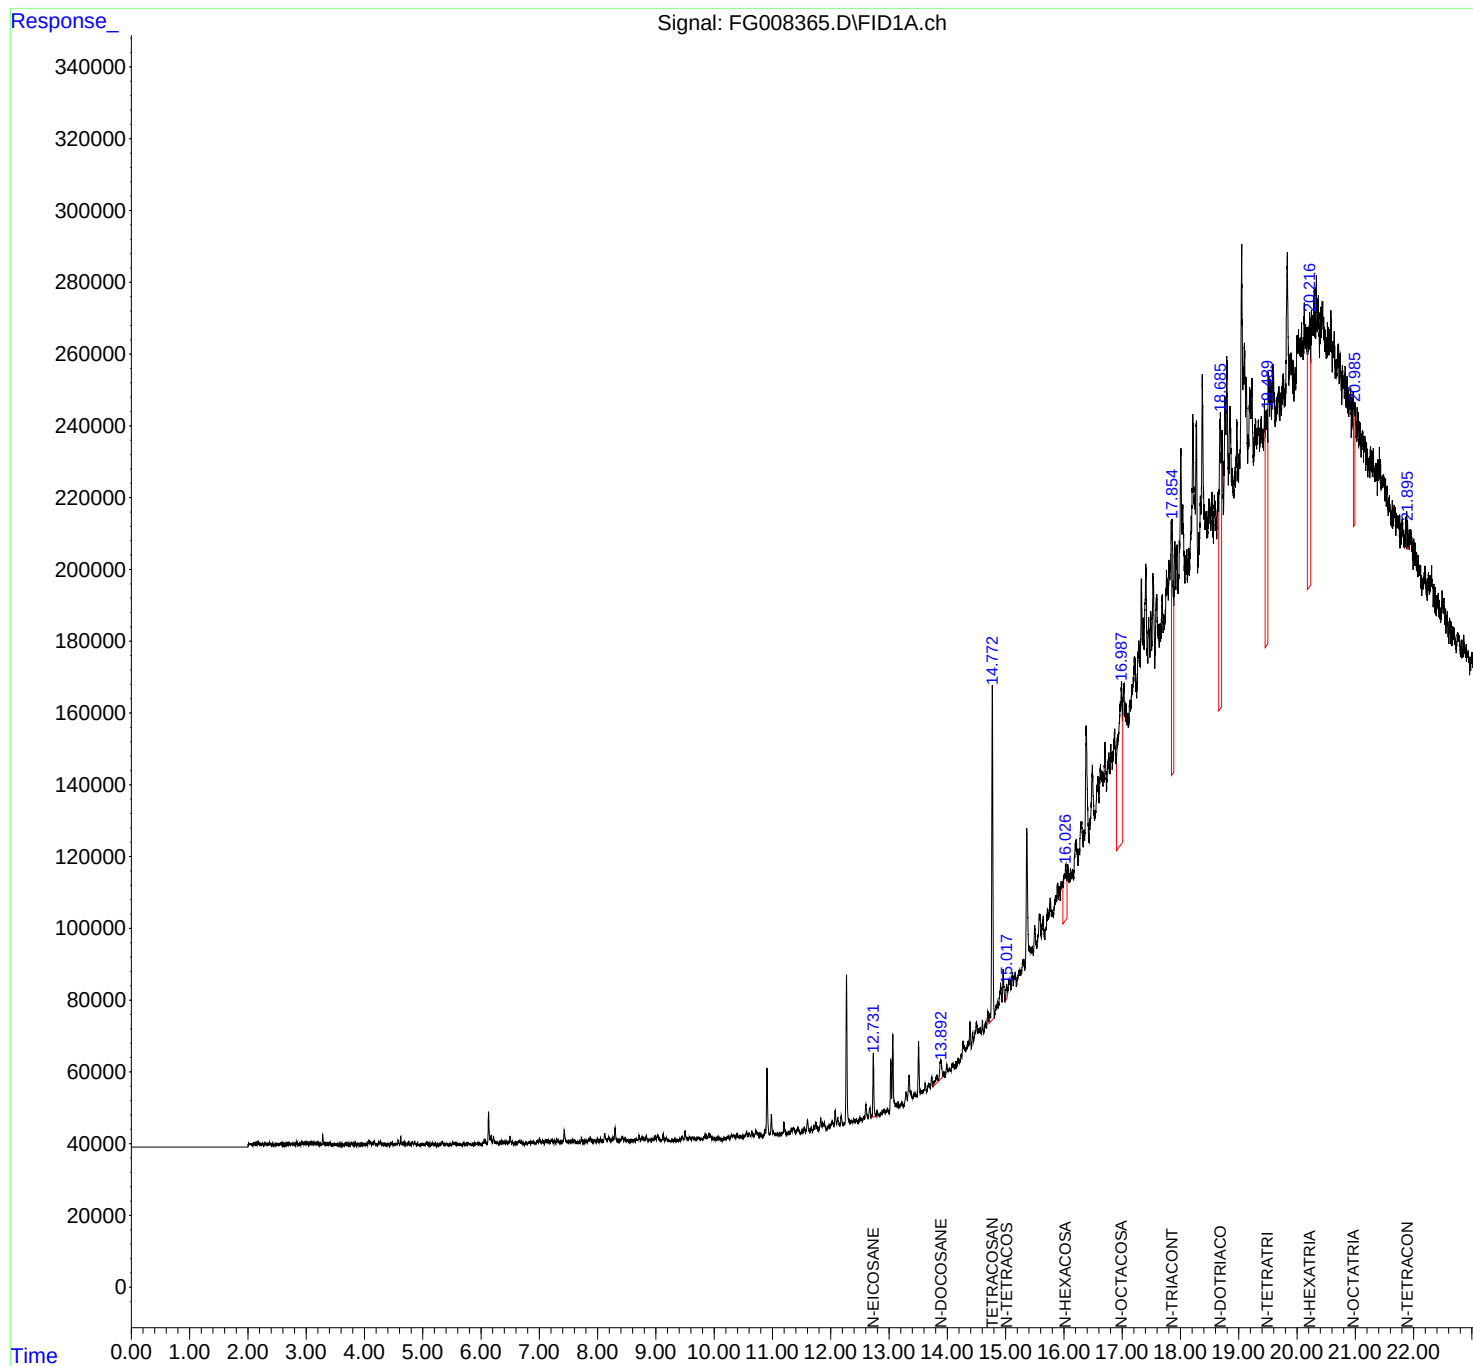


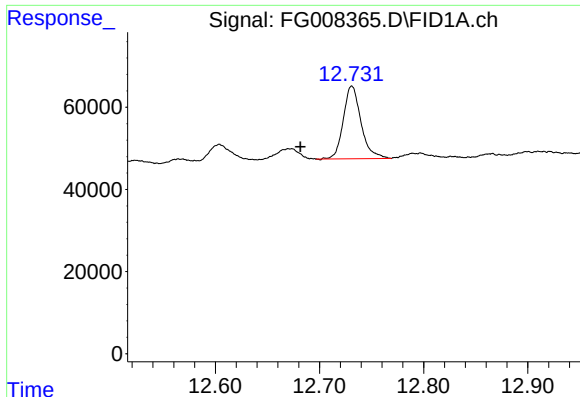

#7 N-EICOSANE


R.T.: 12.731 min
Delta R.T.: 0.050 min
Response: 209590
Conc: 1.53 ug/ml

Instrument :
FID_G
ClientSampleId :

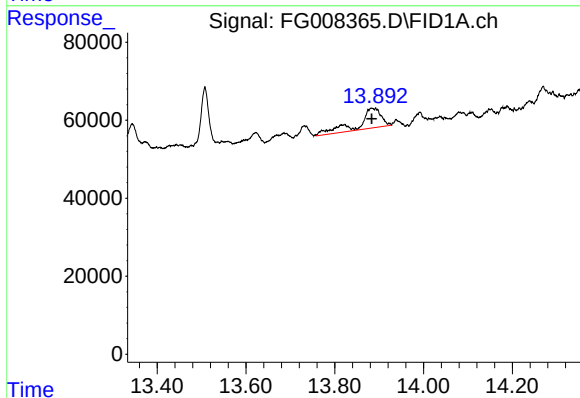


#8 N-DOCOSANE

R.T.: 13.892 min
Delta R.T.: 0.009 min
Response: 180593
Conc: 1.33 ug/ml

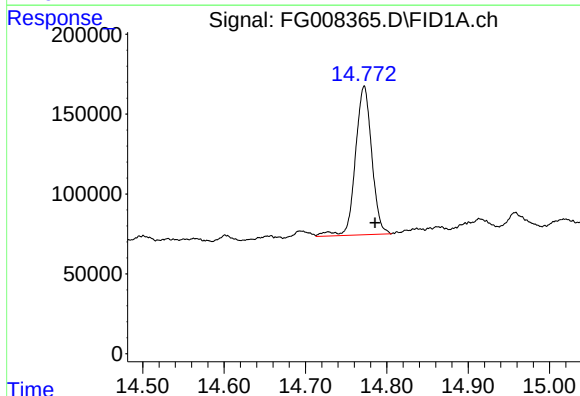


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.772 min
Delta R.T.: -0.013 min
Response: 1296272
Conc: 10.92 ug/ml

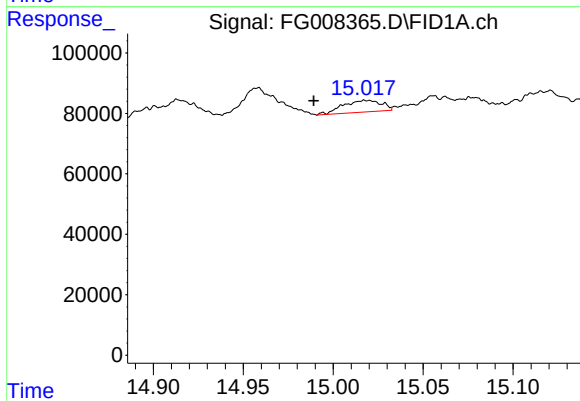

#10 N-TETRACOSANE


R.T.: 15.019 min
Delta R.T.: 0.029 min
Response: 57733
Conc: 0.43 ug/ml

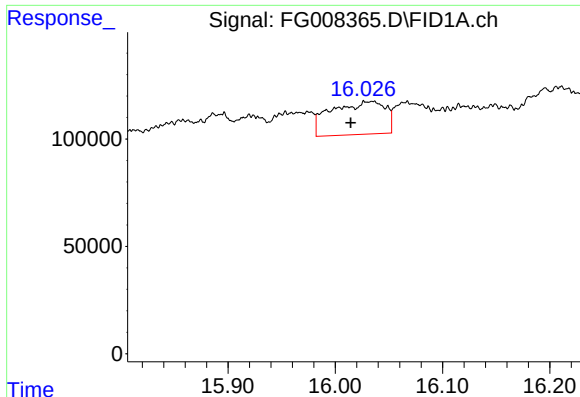

#11 N-HEXACOSANE


R.T.: 16.028 min
Delta R.T.: 0.013 min
Response: 540019
Conc: 4.11 ug/ml

Instrument :
FID_G
ClientSampleId :

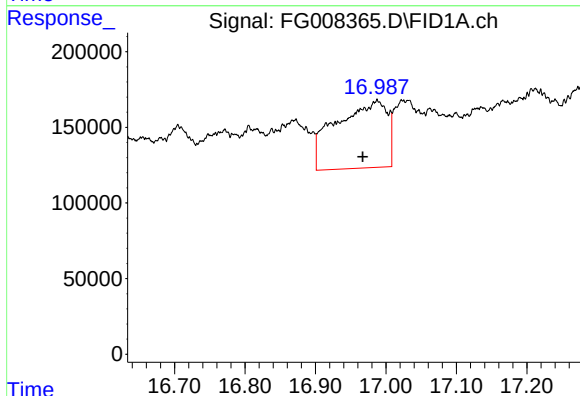


#12 N-OCTACOSANE

R.T.: 16.988 min
Delta R.T.: 0.020 min
Response: 2238074
Conc: 17.27 ug/ml

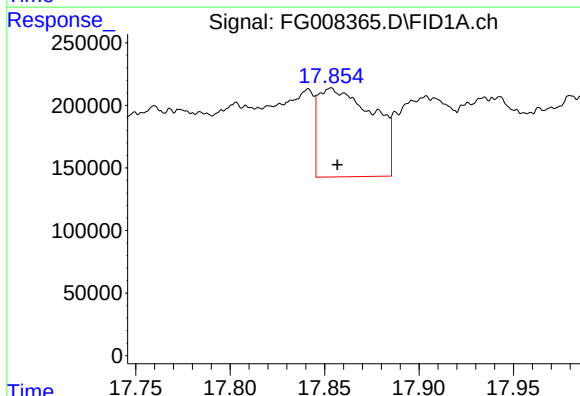


#13 N-TRIACONTANE

R.T.: 17.853 min
Delta R.T.: -0.004 min
Response: 1433139
Conc: 11.23 ug/ml

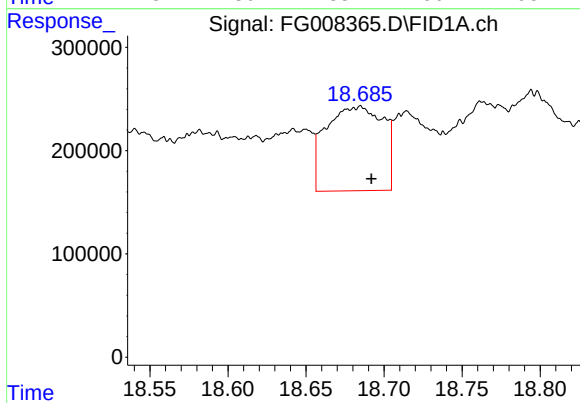

#14 N-DOTRIACONTANE


R.T.: 18.685 min
Delta R.T.: -0.007 min
Response: 2075264
Conc: 16.70 ug/ml

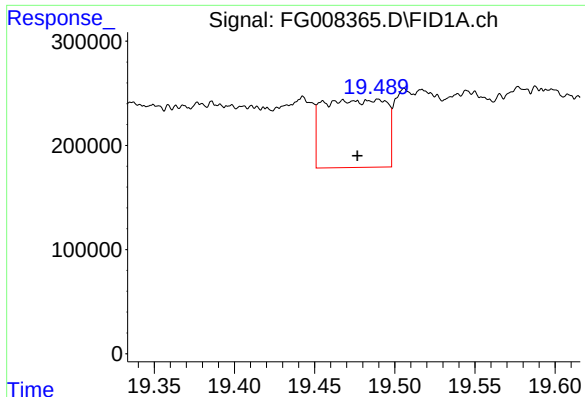

#15 N-TETRATRIACONTANE


R.T.: 19.490 min
Delta R.T.: 0.013 min
Response: 1779146
Conc: 15.21 ug/ml

Instrument :
FID_G
ClientSampleId :

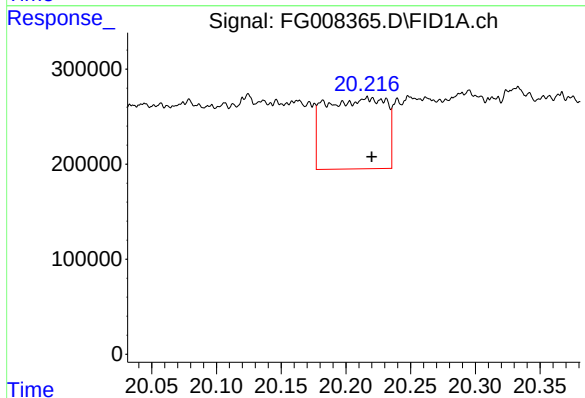


#16 N-HEXATRIACONTANE

R.T.: 20.220 min
Delta R.T.: 0.000 min
Response: 2450493
Conc: 22.13 ug/ml

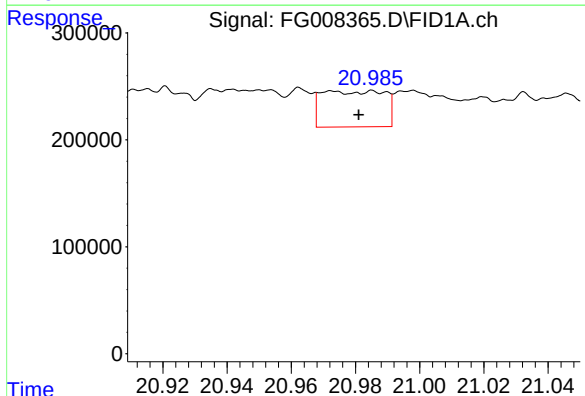

#17 N-OCTATRIACONTANE

R.T.: 20.973 min
Delta R.T.: -0.008 min
Response: 456311
Conc: 4.42 ug/ml

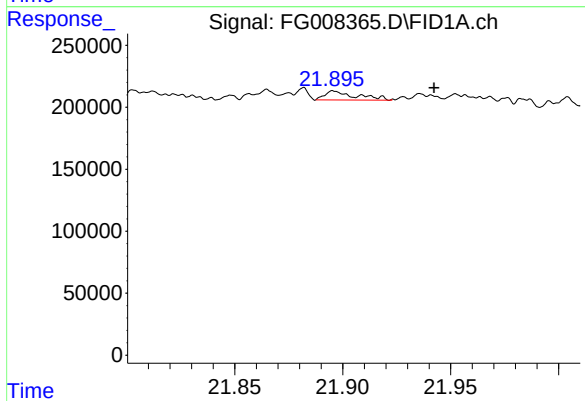

#18 N-TETRACONTANE

R.T.: 21.896 min
Delta R.T.: -0.046 min
Response: 72756
Conc: 0.68 ug/ml