

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061918\
Data File : FG001368.D
Signal(s) : FID1A.ch
Acq On : 19 Jun 2018 11:34
Operator : UA\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 07:53:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.289	3794030	27.368 ug/ml
12)	N-OCTACOSANE	16.710	3462478	25.095 ug/ml
13)	N-TRIACONTANE	17.598	247049	1.800 ug/ml
14)	N-DOTRIACONTANE	18.432	355958	2.661 ug/ml
15)	N-TETRATRIACONTANE	19.220	265466	2.015 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061918\
Data File : FG001368.D
Signal(s) : FID1A.ch
Acq On : 19 Jun 2018 11:34
Operator : UA\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 07:53:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

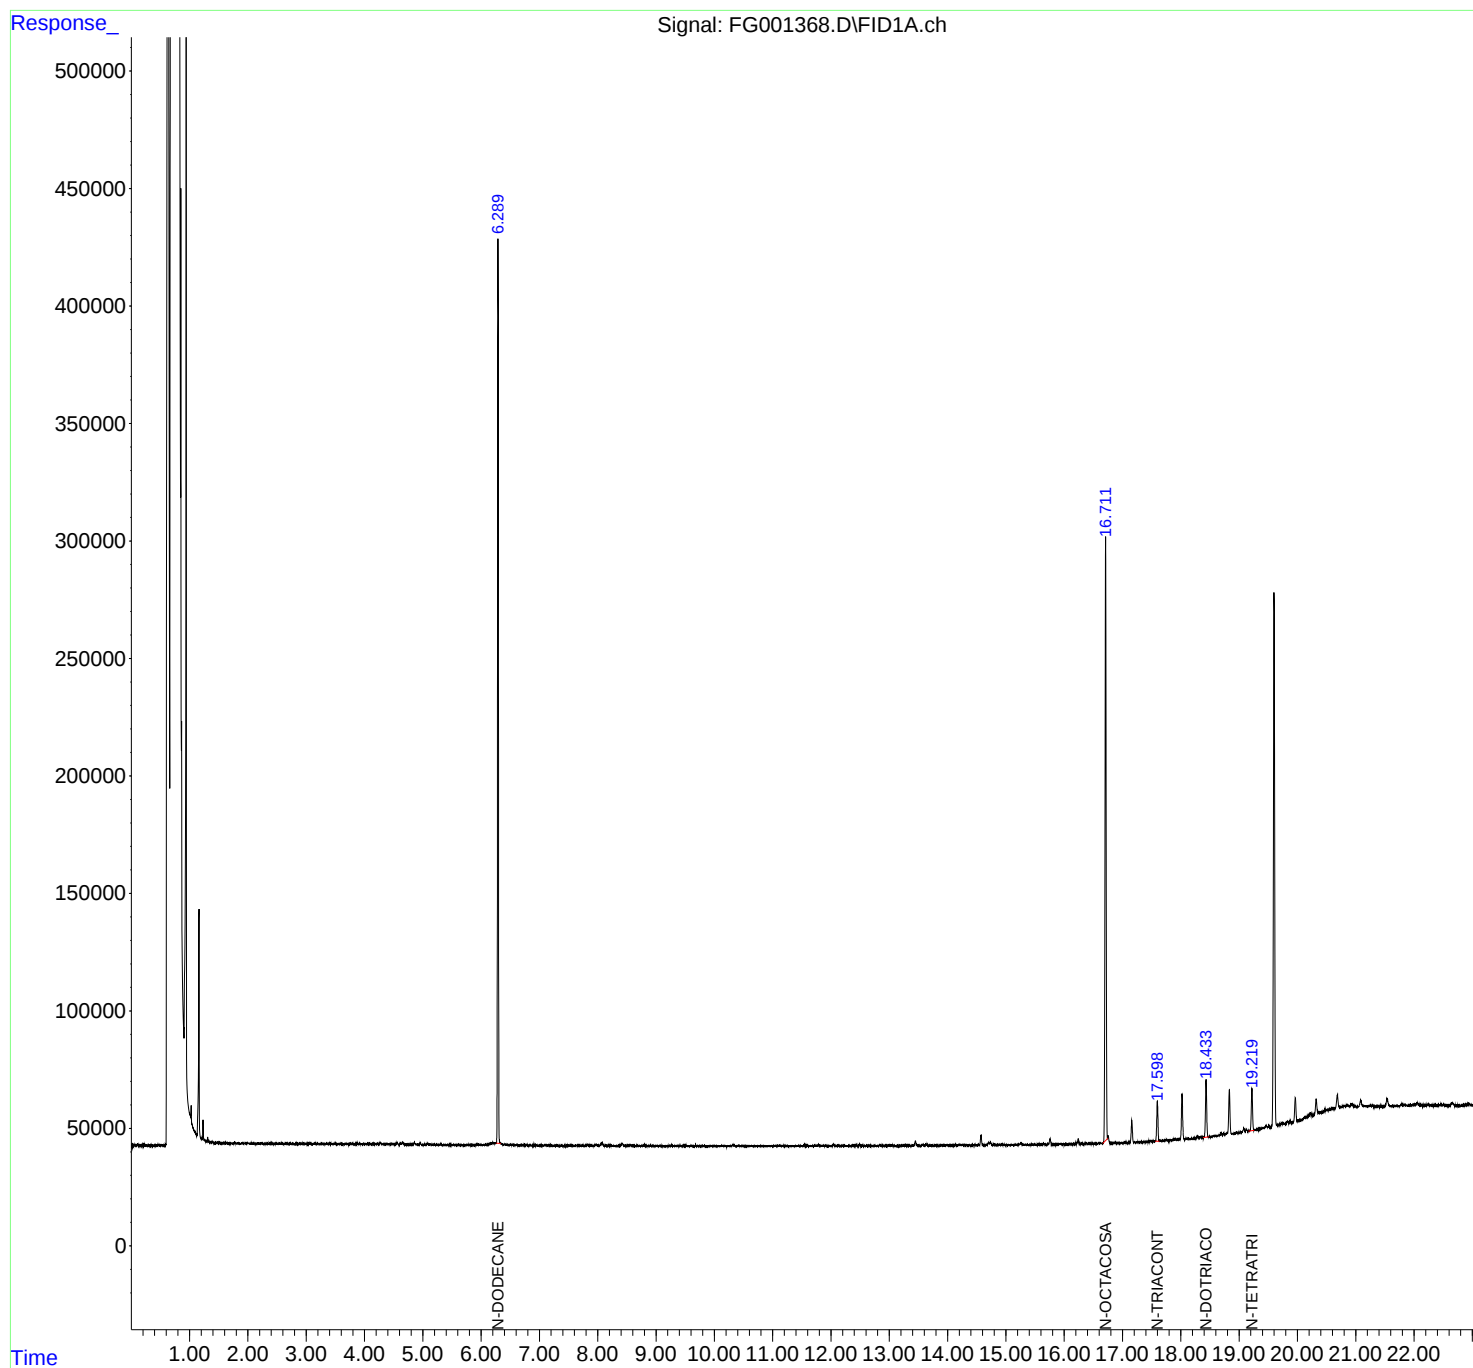


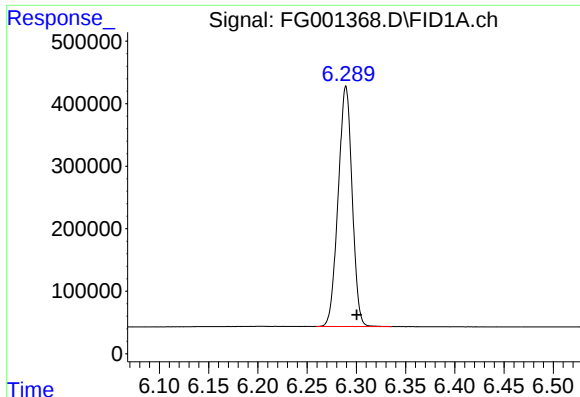

#3 N-DODECANE


R.T.: 6.289 min
Delta R.T.: -0.011 min
Response: 3794030
Conc: 27.37 ug/ml

Instrument :
FID_G
ClientSampleId :

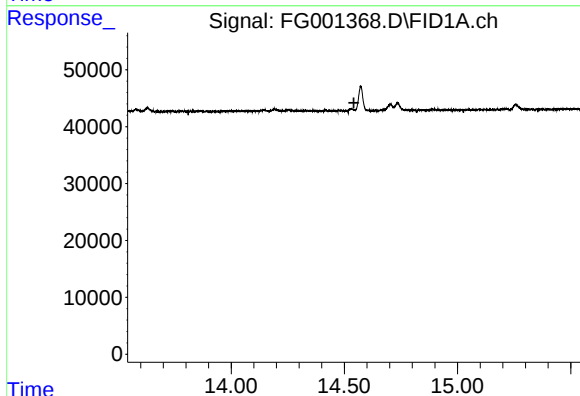


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.542 min
Response: 0
Conc: N.D.

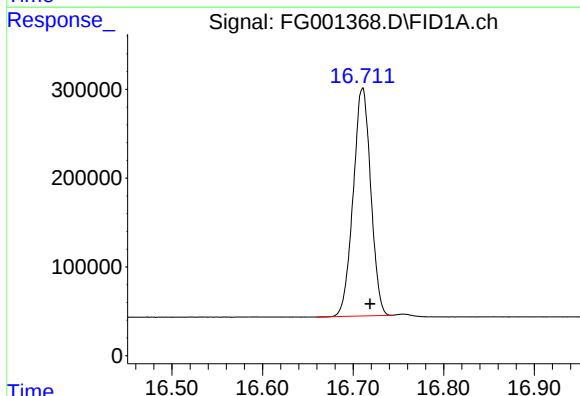


#12 N-OCTACOSANE

R.T.: 16.710 min
Delta R.T.: -0.008 min
Response: 3462478
Conc: 25.09 ug/ml

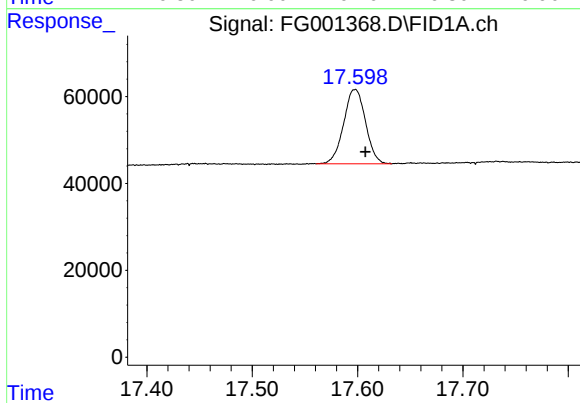

#13 N-TRIACONTANE


R.T.: 17.598 min
Delta R.T.: -0.010 min
Response: 247049
Conc: 1.80 ug/ml

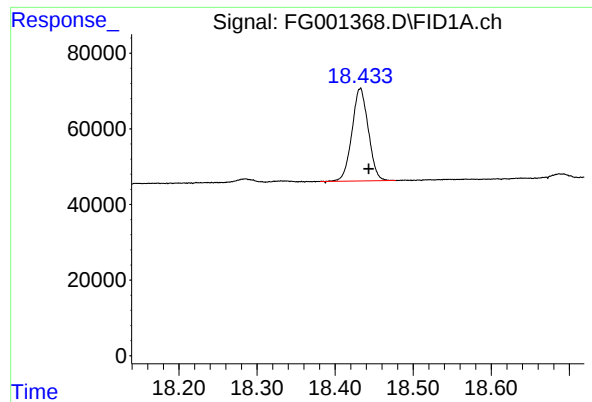

#14 N-DOTRIACONTANE

R.T.: 18.432 min
Delta R.T.: -0.011 min
Response: 355958
Conc: 2.66 ug/ml

Instrument :
FID_G
ClientSampleId :

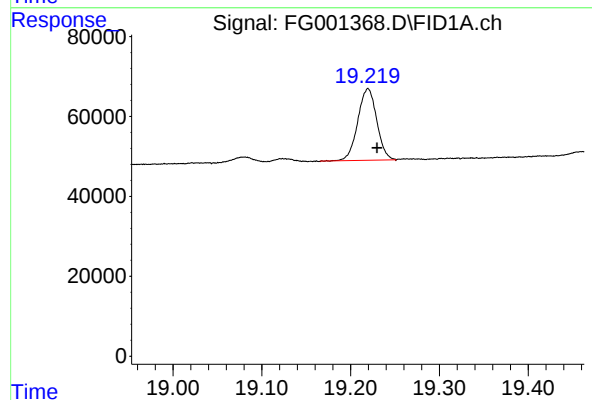

#15 N-TETRATRIACONTANE

R.T.: 19.220 min
Delta R.T.: -0.010 min
Response: 265466
Conc: 2.02 ug/ml