

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061918\
 Data File : FG001377.D
 Signal(s) : FID1A.ch
 Acq On : 19 Jun 2018 17:20
 Operator : UA\AJ
 Sample : J3575-09 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 07:55:30 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.537	1139797	9.324 ug/ml
Target Compounds			
4) N-TETRADECANE	8.139	155743	1.115 ug/ml
7) N-EICOSANE	12.432	698334	4.959 ug/ml
8) N-DOCOSANE	13.650	1754220	12.517 ug/ml
10) N-TETRACOSANE	14.753	306906	2.207 ug/ml
11) N-HEXACOSANE	15.772	448638	3.239 ug/ml
12) N-OCTACOSANE	16.712	792696	5.745 ug/ml
13) N-TRIACONTANE	17.604	429757	3.132 ug/ml
14) N-DOTRIACONTANE	18.374f	763185	5.706 ug/ml
16) N-HEXATRIACONTANE	19.928	311717	2.480 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061918\
Data File : FG001377.D
Signal(s) : FID1A.ch
Acq On : 19 Jun 2018 17:20
Operator : UA\AJ
Sample : J3575-09 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 07:55:30 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

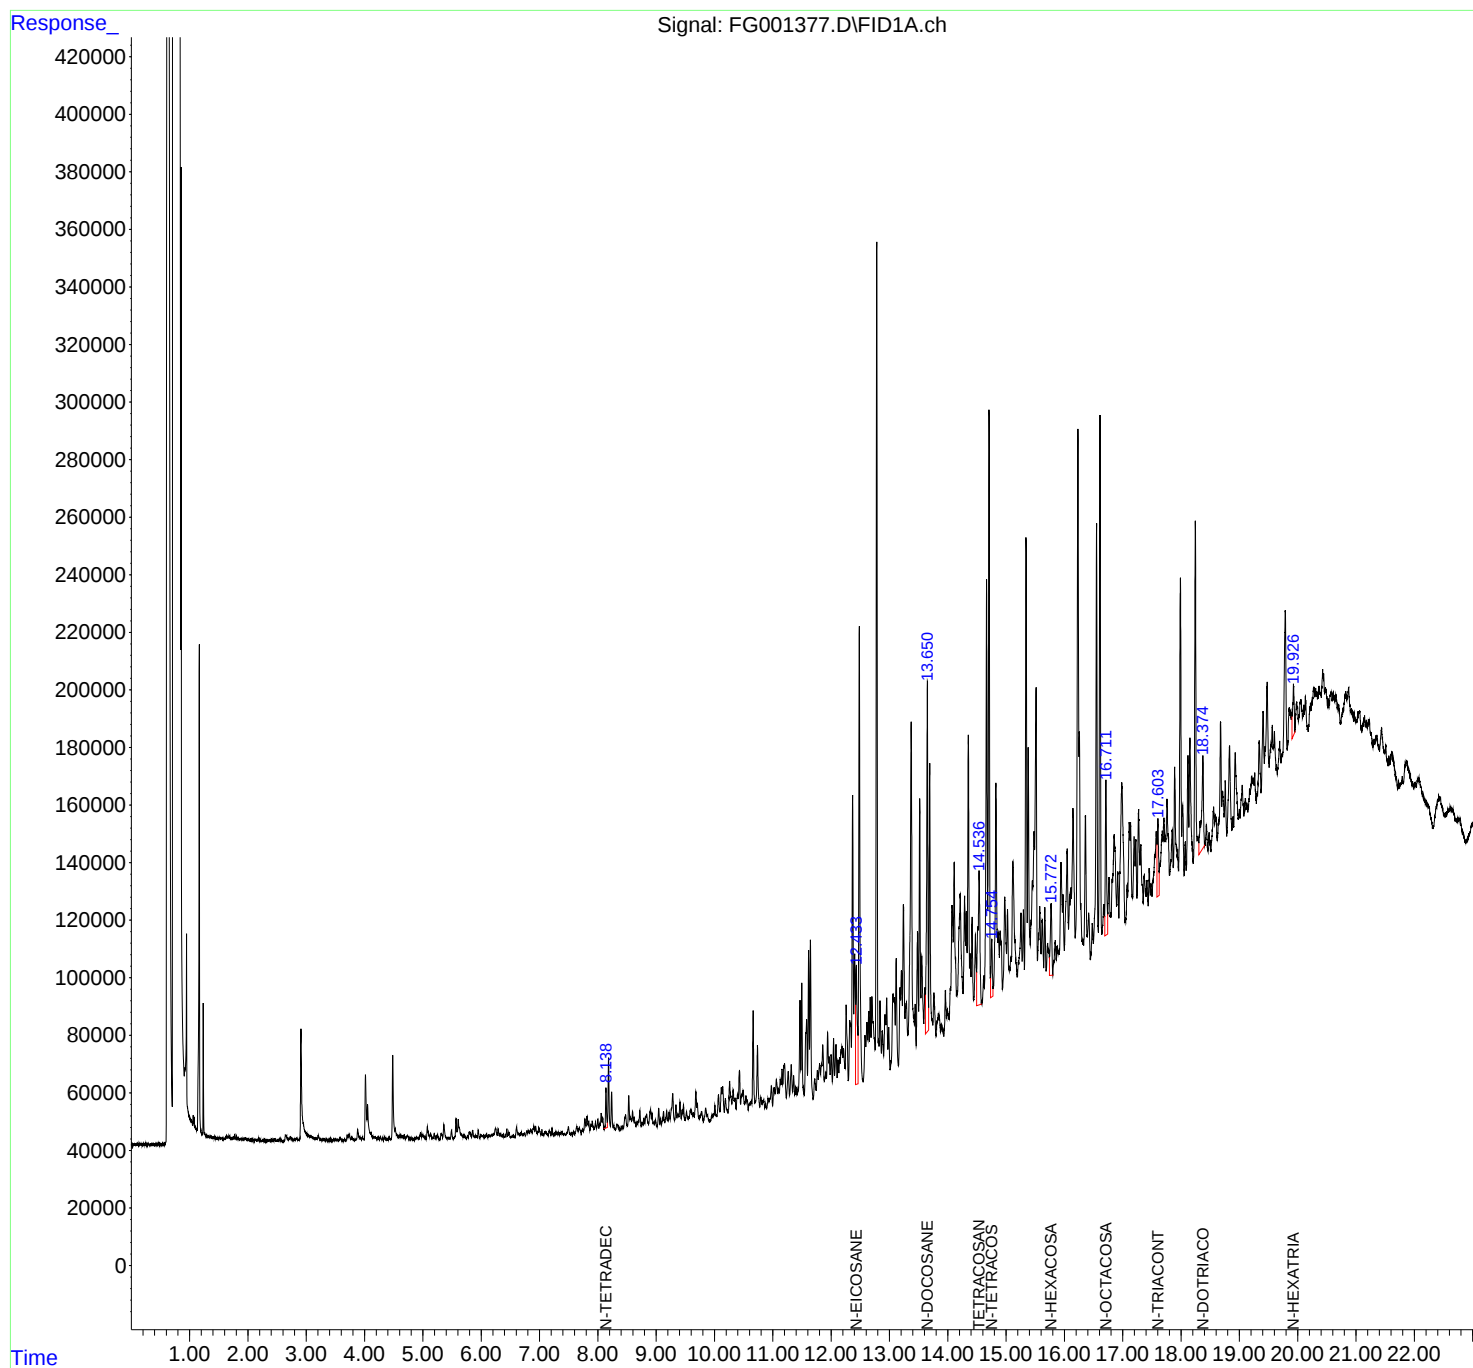


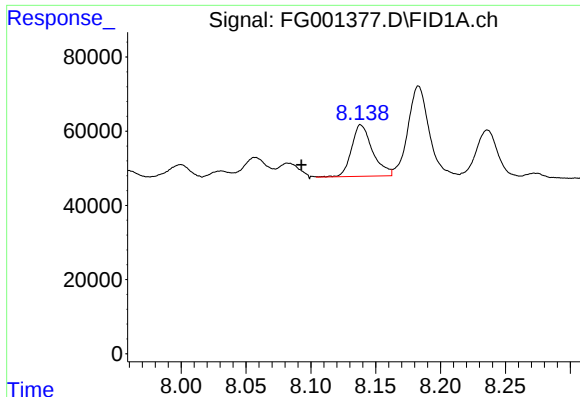

#4 N-TETRADECANE


R.T.: 8.139 min
Delta R.T.: 0.046 min
Response: 155743
Conc: 1.11 ug/ml

Instrument :
FID_G
ClientSampleId :

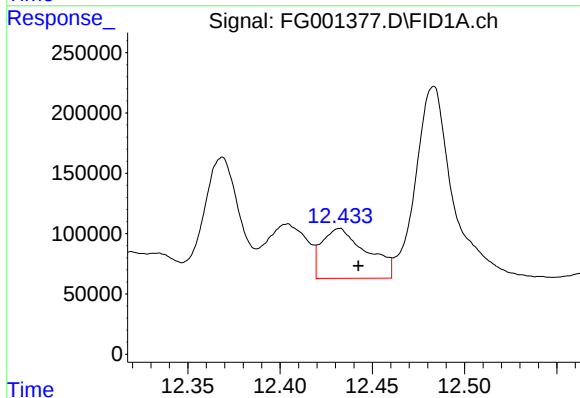


#7 N-EICOSANE

R.T.: 12.432 min
Delta R.T.: -0.010 min
Response: 698334
Conc: 4.96 ug/ml

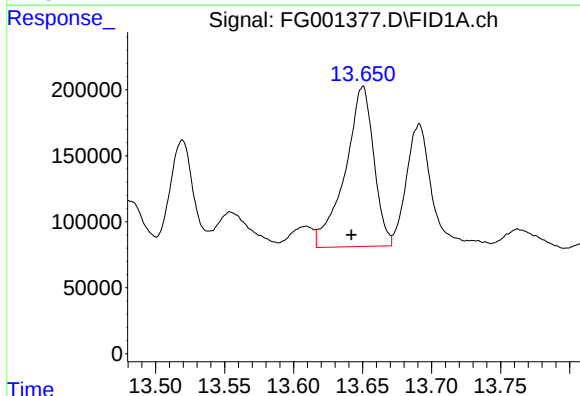


#8 N-DOCOSANE

R.T.: 13.650 min
Delta R.T.: 0.008 min
Response: 1754220
Conc: 12.52 ug/ml

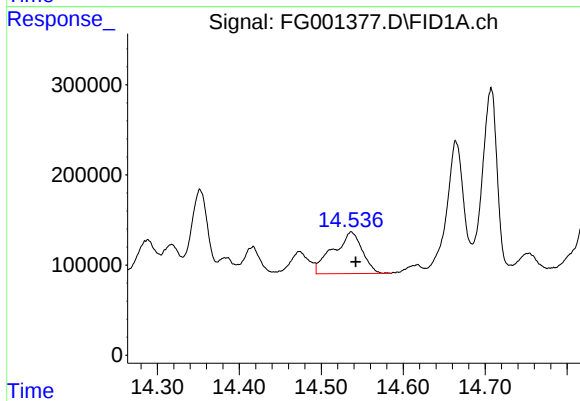

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.537 min
Delta R.T.: -0.006 min
Response: 1139797
Conc: 9.32 ug/ml

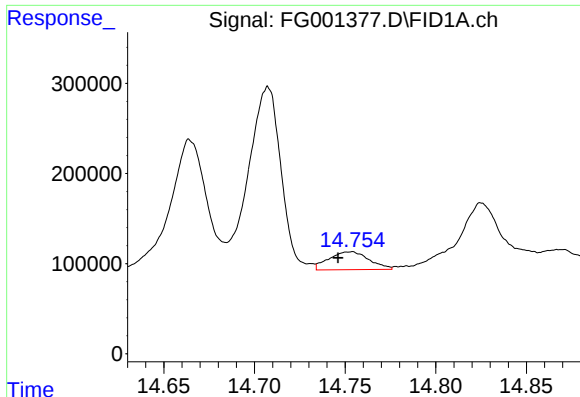

#10 N-TETRACOSANE


R.T.: 14.753 min
Delta R.T.: 0.007 min
Response: 306906
Conc: 2.21 ug/ml

Instrument :
FID_G
ClientSampleId :

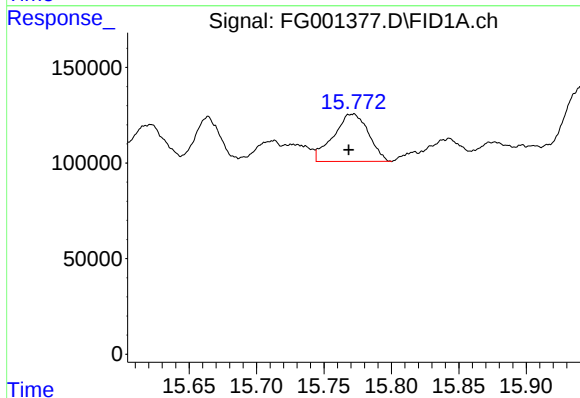


#11 N-HEXACOSANE

R.T.: 15.772 min
Delta R.T.: 0.003 min
Response: 448638
Conc: 3.24 ug/ml

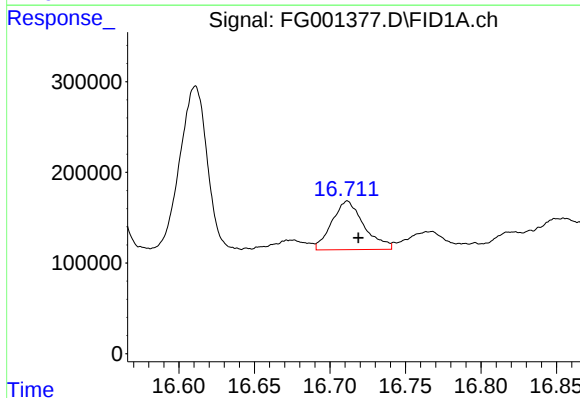


#12 N-OCTACOSANE

R.T.: 16.712 min
Delta R.T.: -0.007 min
Response: 792696
Conc: 5.75 ug/ml

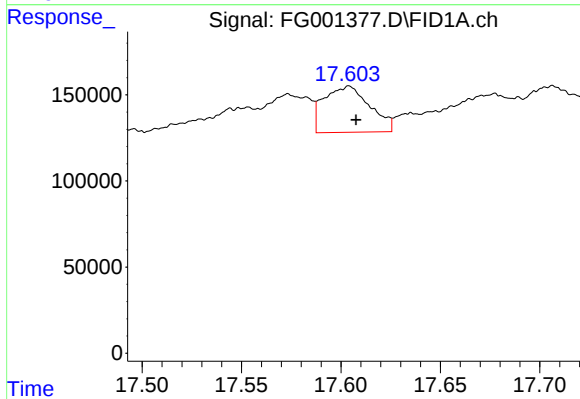

#13 N-TRIACONTANE


R.T.: 17.604 min
Delta R.T.: -0.003 min
Response: 429757
Conc: 3.13 ug/ml

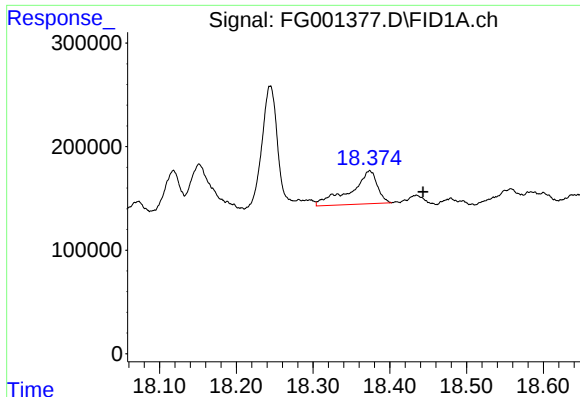

#14 N-DOTRIACONTANE

R.T.: 18.374 min
Delta R.T.: -0.069 min
Response: 763185
Conc: 5.71 ug/ml

Instrument :
FID_G
ClientSampleId :

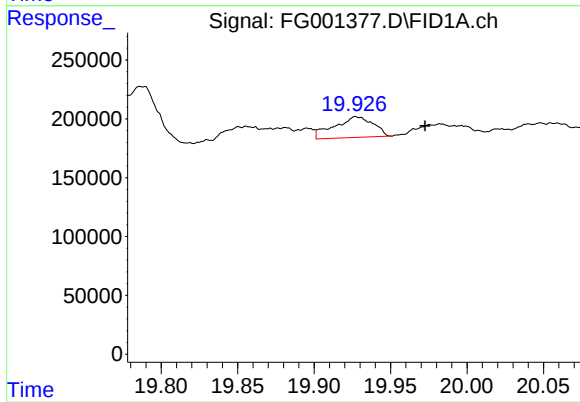

#16 N-HEXATRIACONTANE

R.T.: 19.928 min
Delta R.T.: -0.045 min
Response: 311717
Conc: 2.48 ug/ml