

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061918\  
Data File : FG001390.D  
Signal(s) : FID1A.ch  
Acq On : 19 Jun 2018 23:55  
Operator : UA\AJ  
Sample : J3497-01  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 20 07:57:46 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_G\Method\FG060118.M  
Quant Title :  
QLast Update : Fri Jun 01 15:28:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |               | R.T.   | Response | Conc Units  |
|-----------------------------|---------------|--------|----------|-------------|
| -----                       |               |        |          |             |
| System Monitoring Compounds |               |        |          |             |
| Target Compounds            |               |        |          |             |
| 4)                          | N-TETRADECANE | 8.081  | 199053   | 1.425 ug/ml |
| 12)                         | N-OCTACOSANE  | 16.691 | 545970   | 3.957 ug/ml |
| -----                       |               |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG061918\  
Data File : FG001390.D  
Signal(s) : FID1A.ch  
Acq On : 19 Jun 2018 23:55  
Operator : UA\AJ  
Sample : J3497-01  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 20 07:57:46 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_G\Method\FG060118.M  
Quant Title :  
QLast Update : Fri Jun 01 15:28:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

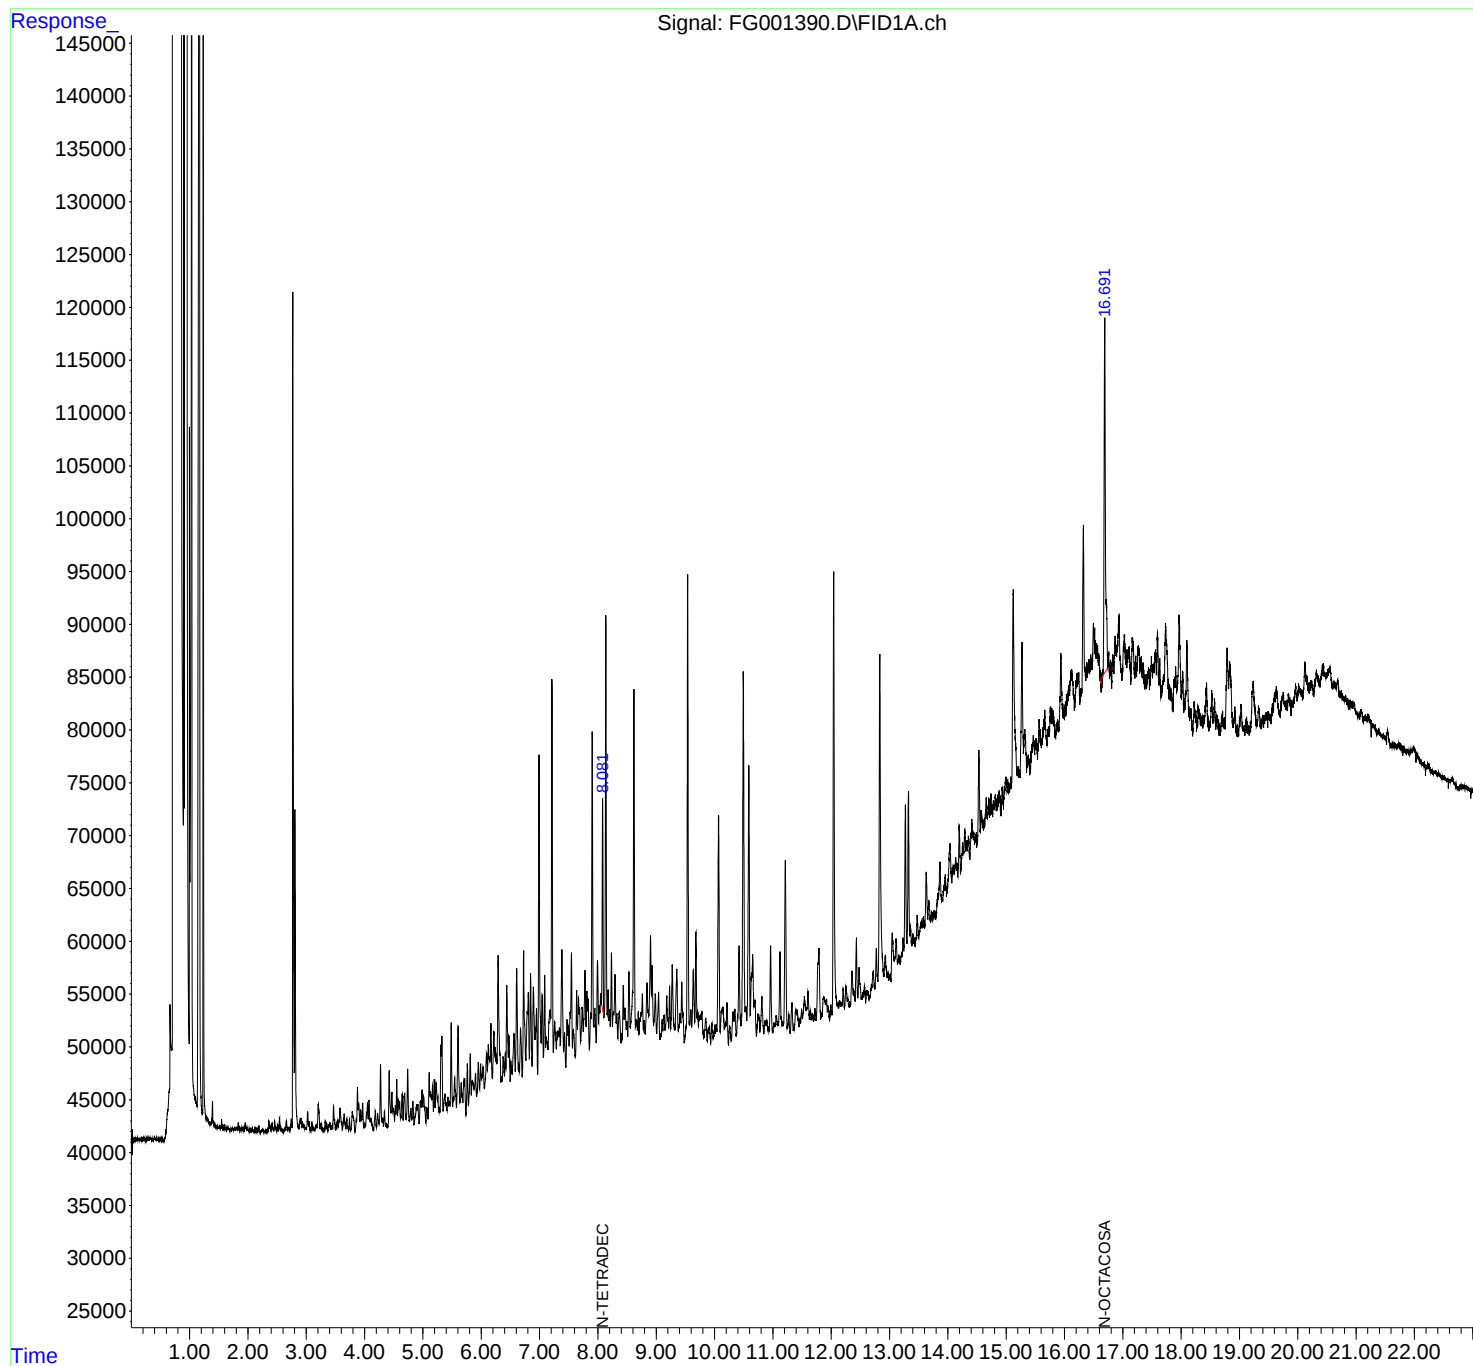


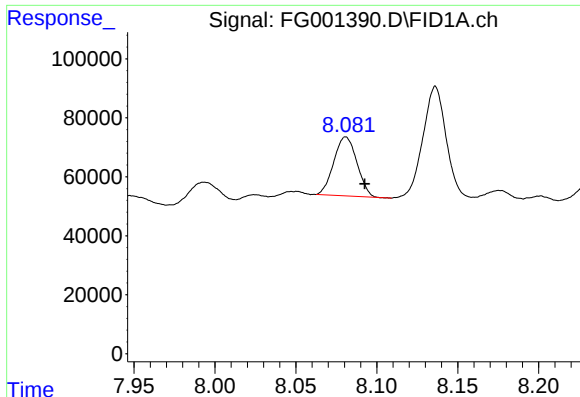

#4 N-TETRADECANE


R.T.: 8.081 min  
Delta R.T.: -0.012 min  
Response: 199053  
Conc: 1.42 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

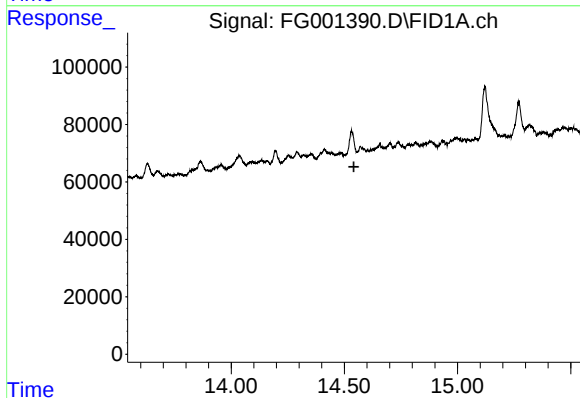

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.542 min  
Response: 0  
Conc: N.D.

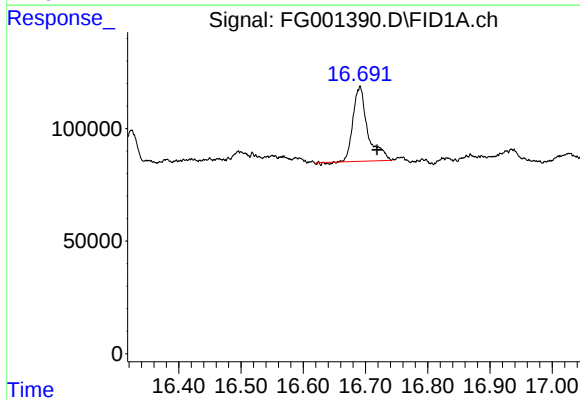

#12 N-OCTACOSANE

R.T.: 16.691 min  
Delta R.T.: -0.027 min  
Response: 545970  
Conc: 3.96 ug/ml