

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061918\
 Data File : FG001370.D
 Signal(s) : FID1A.ch
 Acq On : 19 Jun 2018 13:47
 Operator : UA\AJ
 Sample : PB110377BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 07:54:16 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.531	1627462	13.313 ug/ml
Target Compounds			
2) N-DECANE	4.271	2161805	15.771 ug/ml
3) N-DODECANE	6.287	2164596	15.614 ug/ml
4) N-TETRADECANE	8.079	2153574	15.412 ug/ml
5) N-HEXADECANE	9.679	2122113	15.080 ug/ml
6) N-OCTADECANE	11.121	2108463	14.874 ug/ml
7) N-EICOSANE	12.431	2072168	14.715 ug/ml
8) N-DOCOSANE	13.630	2038071	14.542 ug/ml
10) N-TETRACOSANE	14.735	2028663	14.590 ug/ml
11) N-HEXACOSANE	15.757	1967261	14.201 ug/ml
12) N-OCTACOSANE	16.708	1950277	14.135 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061918\
Data File : FG001370.D
Signal(s) : FID1A.ch
Acq On : 19 Jun 2018 13:47
Operator : UA\AJ
Sample : PB110377BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 07:54:16 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

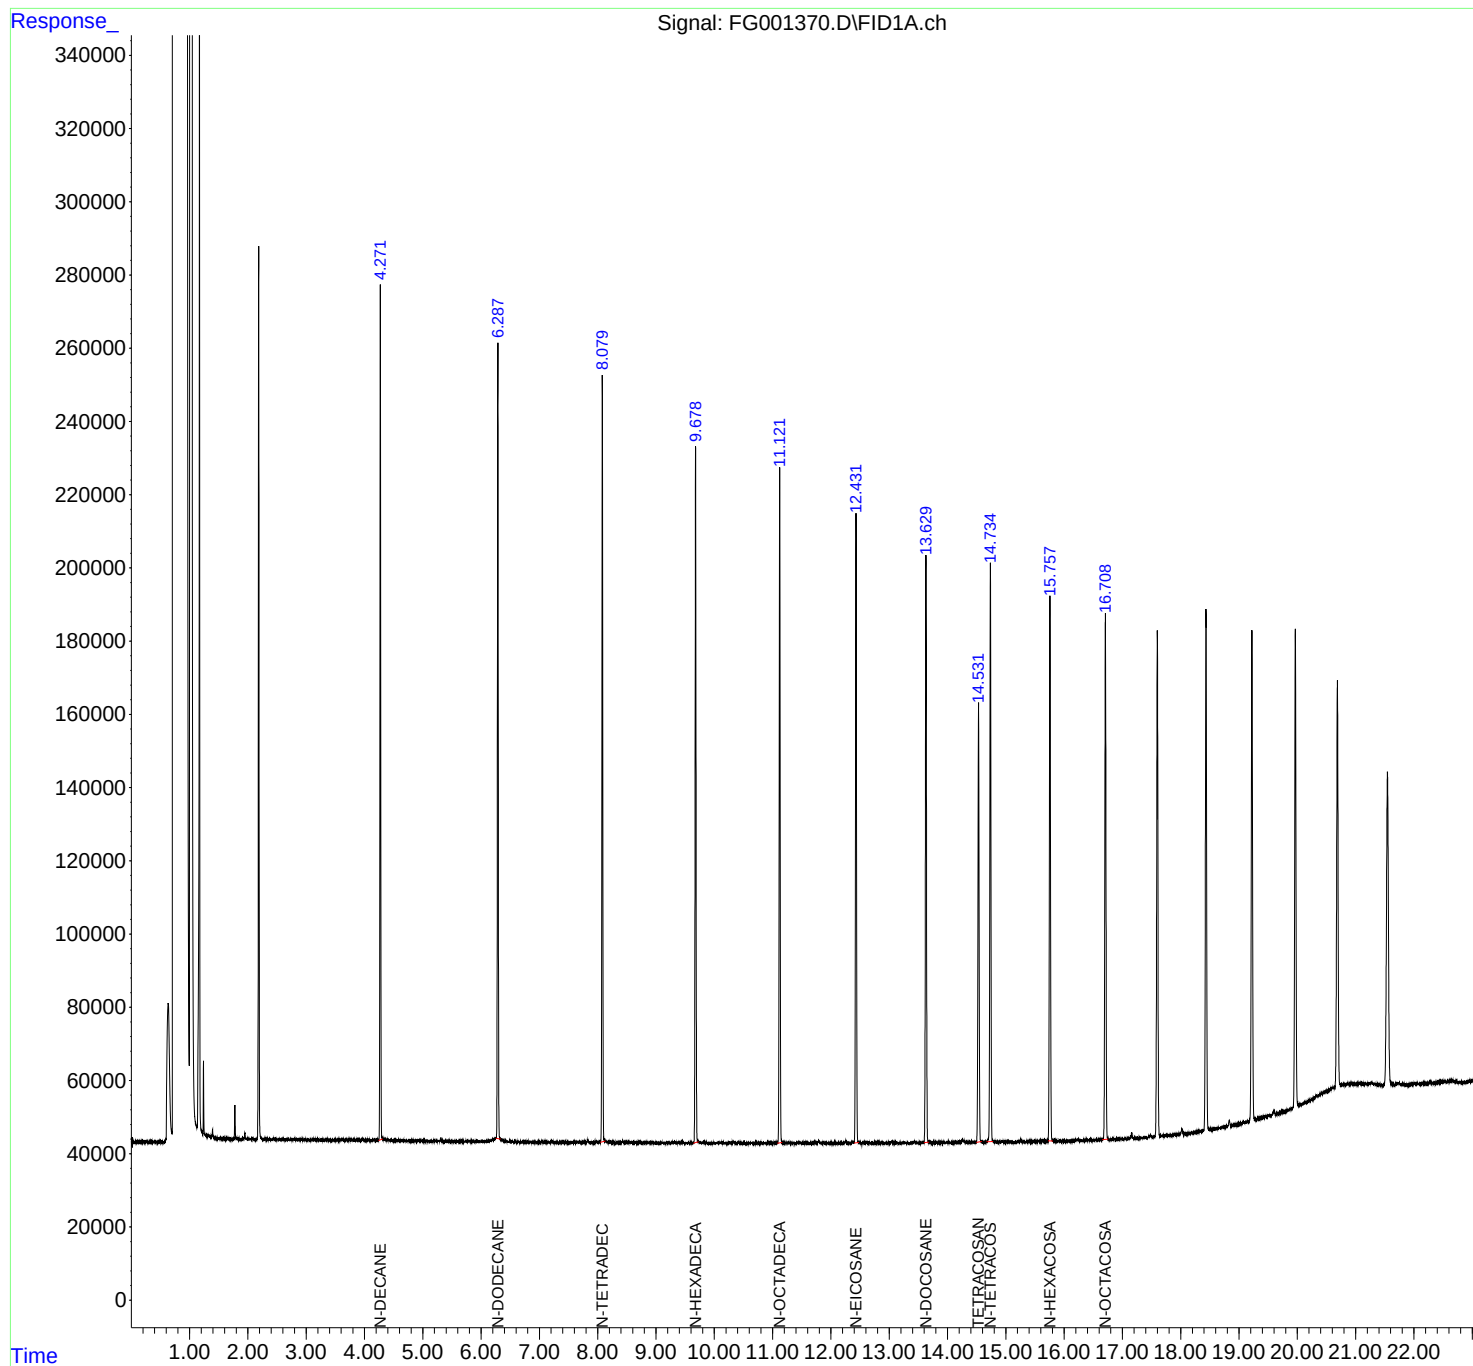


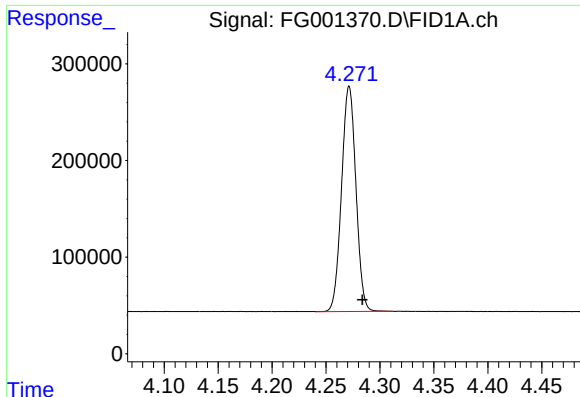

#2 N-DECANE


R.T.: 4.271 min
Delta R.T.: -0.012 min
Response: 2161805
Conc: 15.77 ug/ml

Instrument :
FID_G
ClientSampleId :

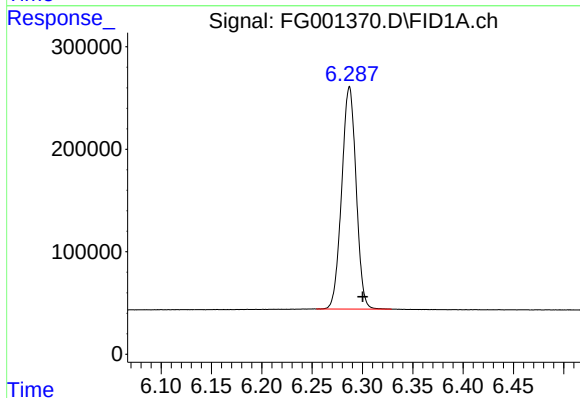


#3 N-DODECANE

R.T.: 6.287 min
Delta R.T.: -0.013 min
Response: 2164596
Conc: 15.61 ug/ml

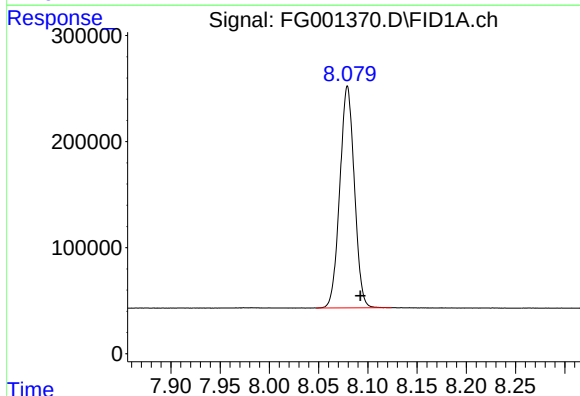


#4 N-TETRADECANE

R.T.: 8.079 min
Delta R.T.: -0.013 min
Response: 2153574
Conc: 15.41 ug/ml

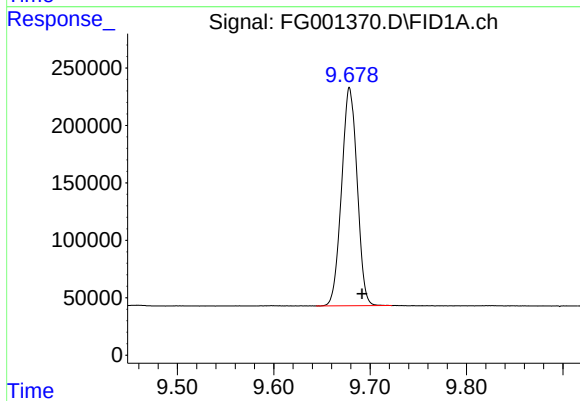

#5 N-HEXADECANE


R.T.: 9.679 min
Delta R.T.: -0.013 min
Response: 2122113
Conc: 15.08 ug/ml

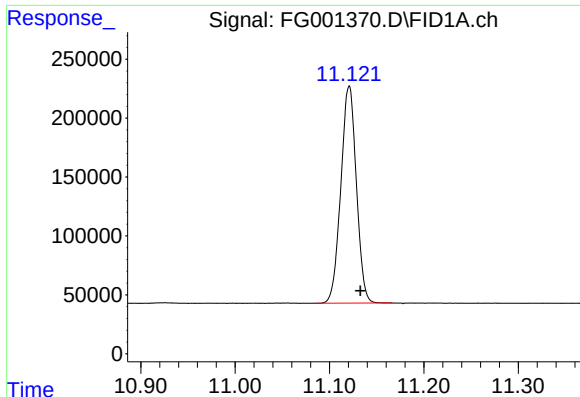

#6 N-OCTADECANE


R.T.: 11.121 min
Delta R.T.: -0.012 min
Response: 2108463
Conc: 14.87 ug/ml

Instrument :
FID_G
ClientSampleId :

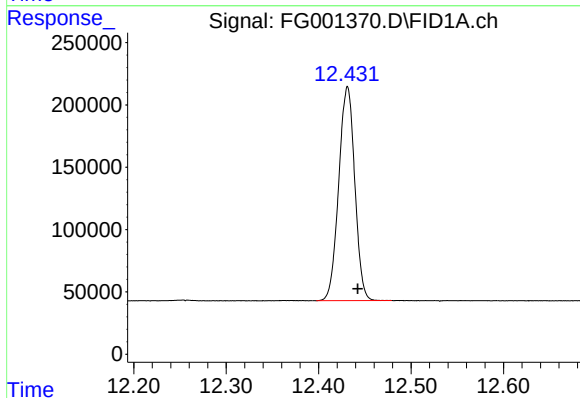


#7 N-EICOSANE

R.T.: 12.431 min
Delta R.T.: -0.011 min
Response: 2072168
Conc: 14.72 ug/ml

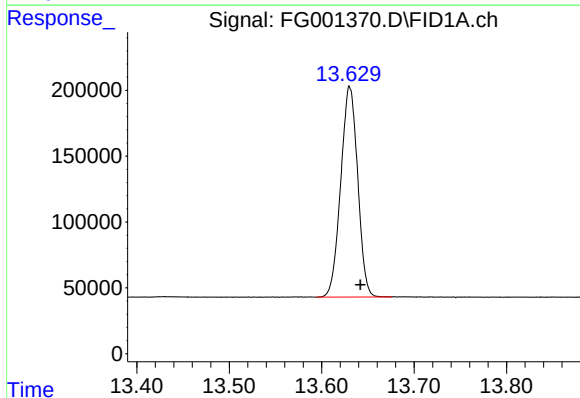


#8 N-DOCOSANE

R.T.: 13.630 min
Delta R.T.: -0.012 min
Response: 2038071
Conc: 14.54 ug/ml

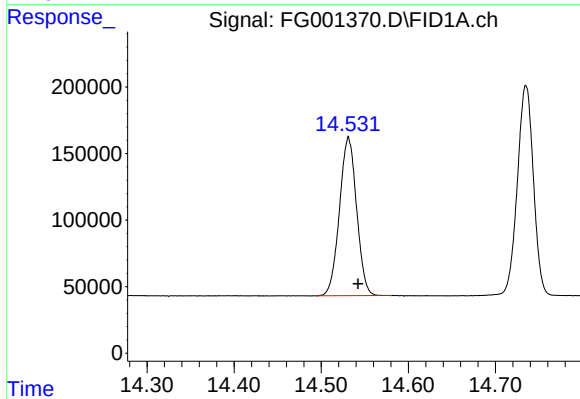

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.531 min
Delta R.T.: -0.011 min
Response: 1627462
Conc: 13.31 ug/ml

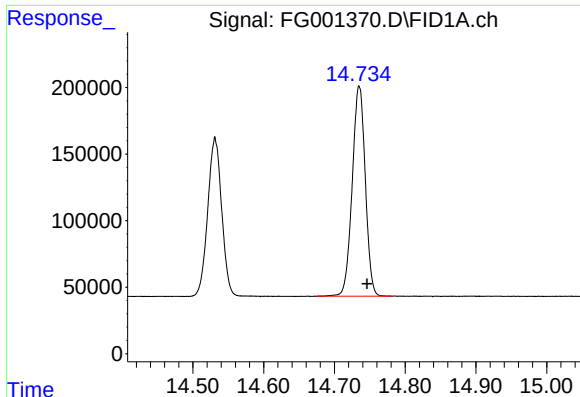

#10 N-TETRACOSANE


R.T.: 14.735 min
Delta R.T.: -0.011 min
Response: 2028663
Conc: 14.59 ug/ml

Instrument :
FID_G
ClientSampleId :

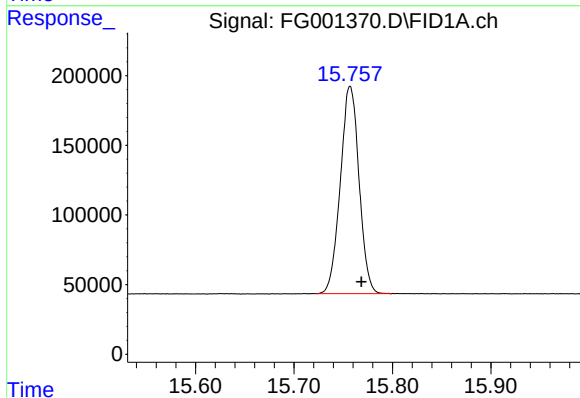

#11 N-HEXACOSANE

R.T.: 15.757 min
Delta R.T.: -0.011 min
Response: 1967261
Conc: 14.20 ug/ml

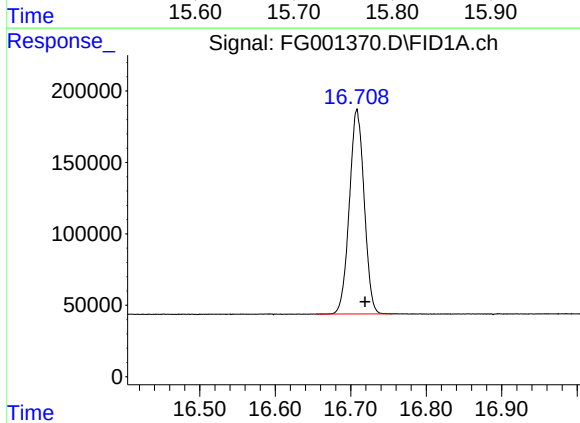

#12 N-OCTACOSANE

R.T.: 16.708 min
Delta R.T.: -0.011 min
Response: 1950277
Conc: 14.13 ug/ml