

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061923\
Data File : FG012214.D
Signal(s) : FID1A.ch
Acq On : 19 Jun 2023 18:10
Operator : YP\AJ
Sample : 03308-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 04:12:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.999	1313250	9.849 ug/ml
Target Compounds			
7) N-EICOSANE	12.962	450674	2.840 ug/ml
10) N-TETRACOSANE	15.186	334266	2.238 ug/ml
14) N-DOTRIACONTANE	18.893	372853	2.921 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061923\
Data File : FG012214.D
Signal(s) : FID1A.ch
Acq On : 19 Jun 2023 18:10
Operator : YP\AJ
Sample : 03308-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 04:12:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

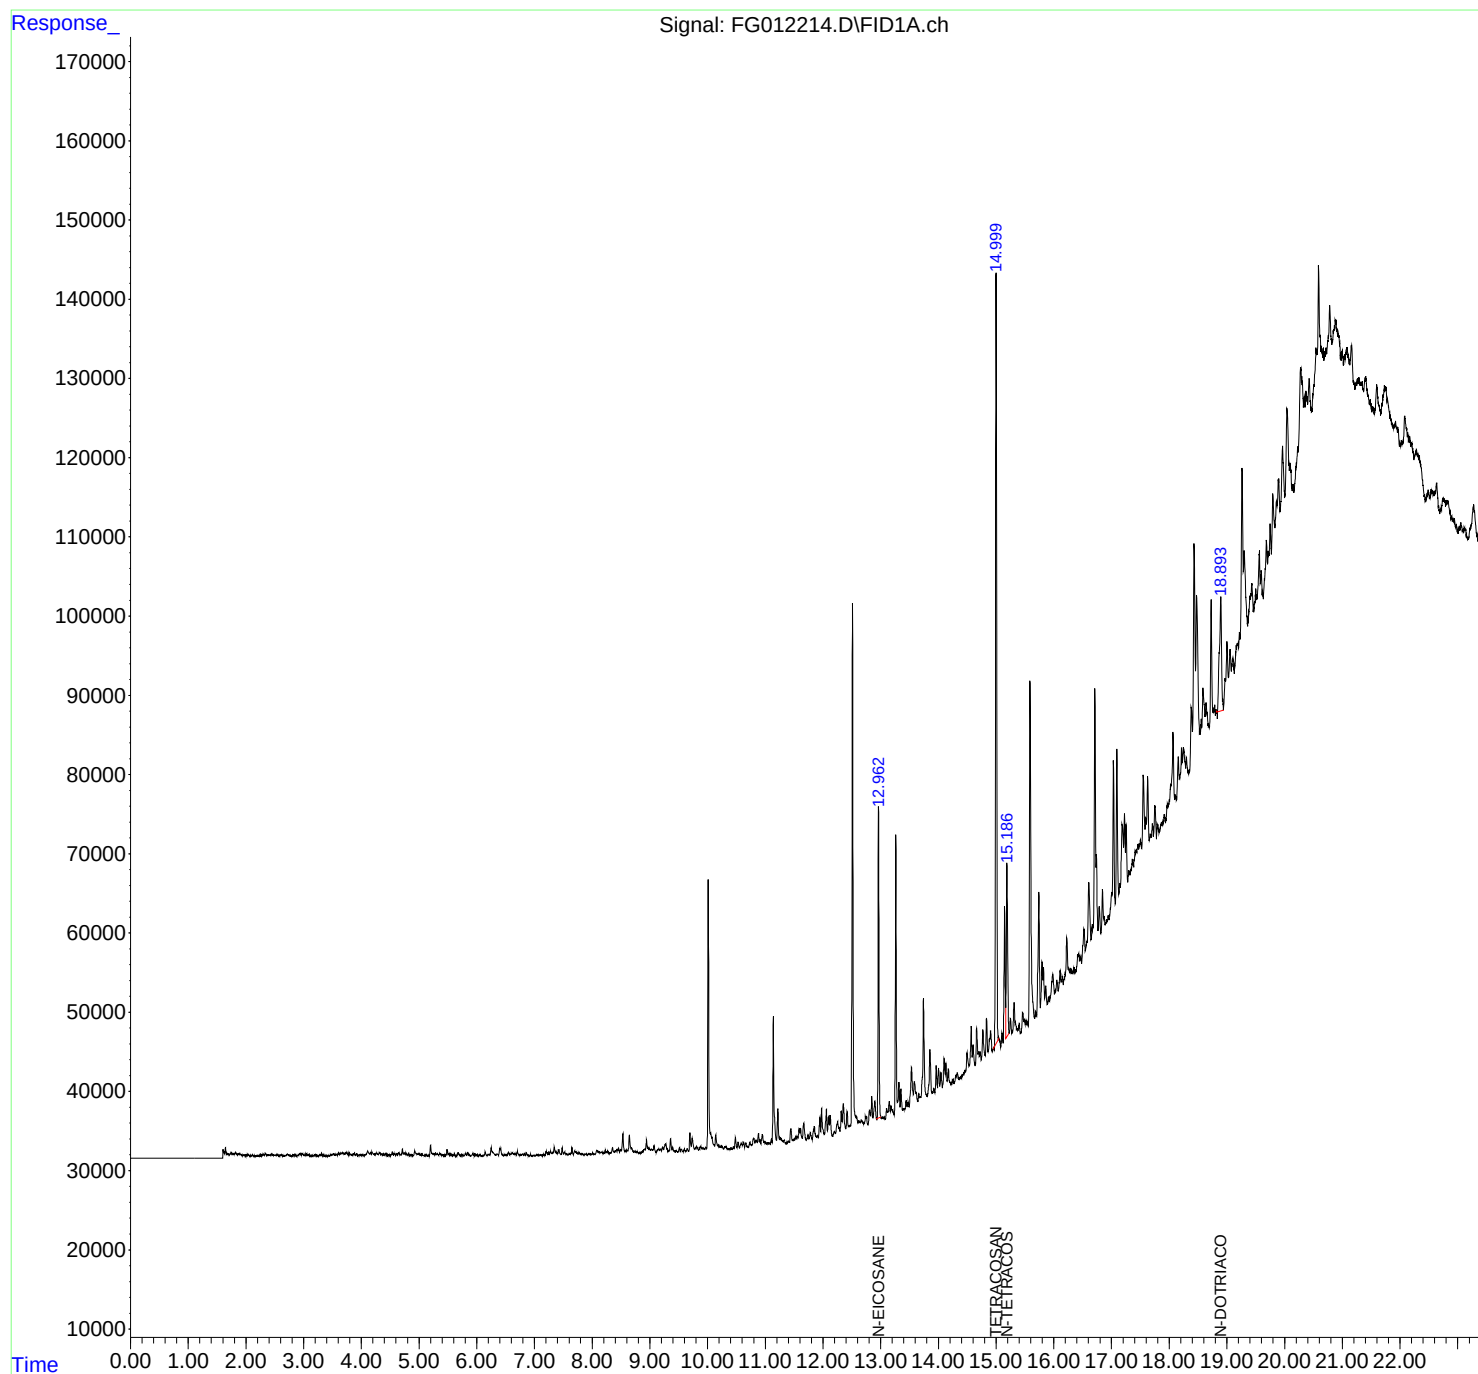


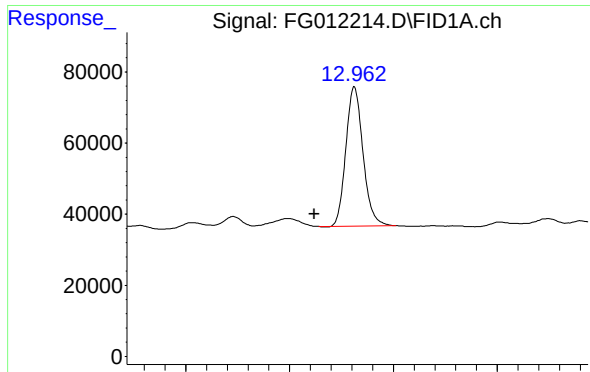

#7 N-EICOSANE


R.T.: 12.962 min
Delta R.T.: 0.039 min
Response: 450674
Conc: 2.84 ug/ml

Instrument :
FID_G
ClientSampleId :

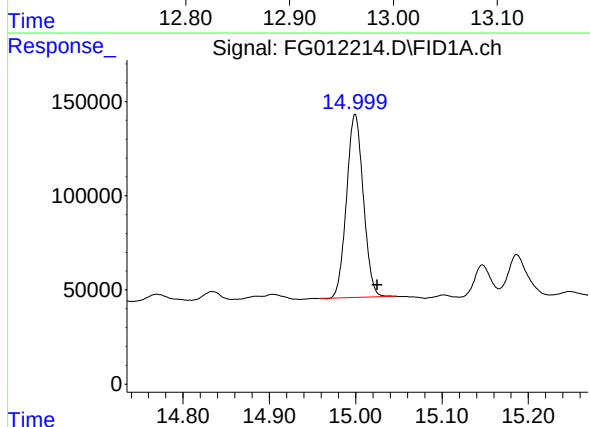


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.999 min
Delta R.T.: -0.026 min
Response: 1313250
Conc: 9.85 ug/ml

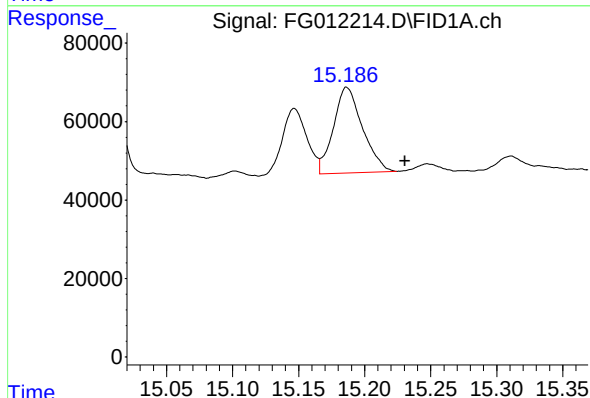

#10 N-TETRACOSANE

R.T.: 15.186 min
Delta R.T.: -0.044 min
Response: 334266
Conc: 2.24 ug/ml

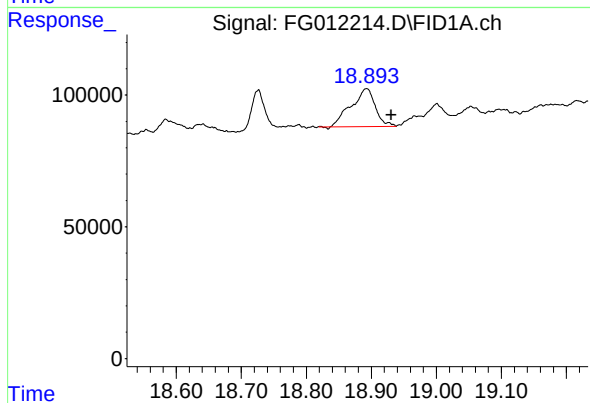

#14 N-DOTRIACONTANE

R.T.: 18.893 min
Delta R.T.: -0.038 min
Response: 372853
Conc: 2.92 ug/ml