

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061923\
 Data File : FG012220.D
 Signal(s) : FID1A.ch
 Acq On : 19 Jun 2023 22:36
 Operator : YP\AJ
 Sample : 03308-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 04:12:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
 Quant Title :
 QLast Update : Thu Jun 01 17:30:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.999	2374786	17.811 ug/ml
Target Compounds			
7) N-EICOSANE	12.963	618899	3.900 ug/ml
10) N-TETRACOSANE	15.186	545764	3.654 ug/ml
13) N-TRIACONTANE	18.067	265314	2.002 ug/ml
14) N-DOTRIACONTANE	18.891	470188	3.684 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061923\
Data File : FG012220.D
Signal(s) : FID1A.ch
Acq On : 19 Jun 2023 22:36
Operator : YP\AJ
Sample : 03308-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 04:12:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

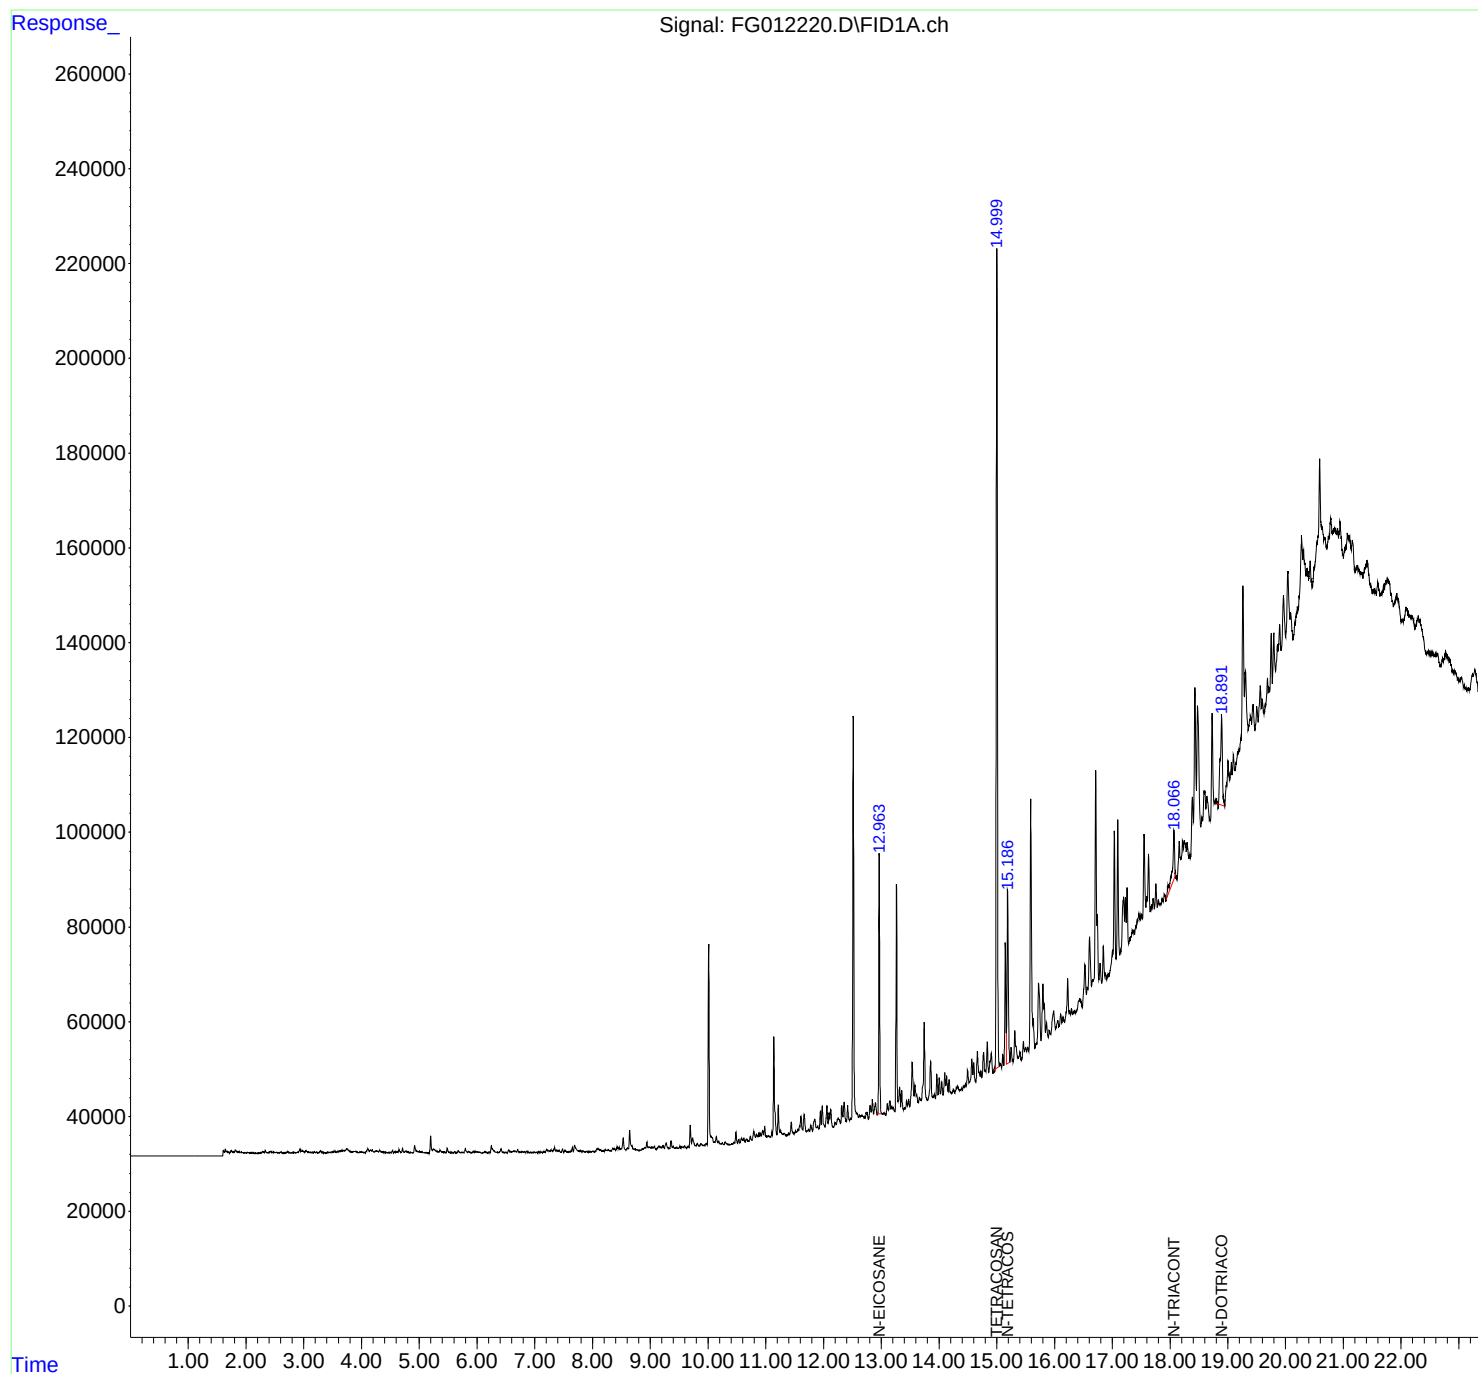


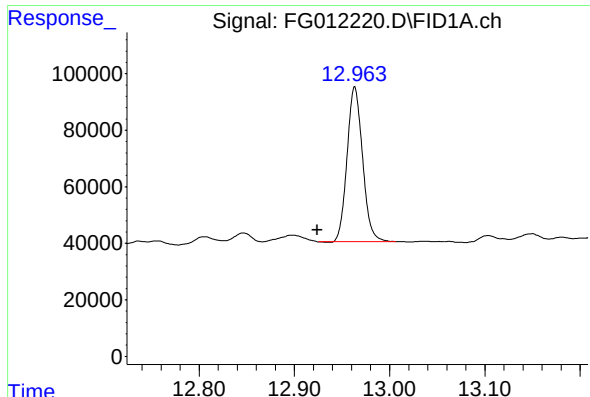

#7 N-EICOSANE


R.T.: 12.963 min
Delta R.T.: 0.040 min
Response: 618899
Conc: 3.90 ug/ml

Instrument :
FID_G
ClientSampleId :

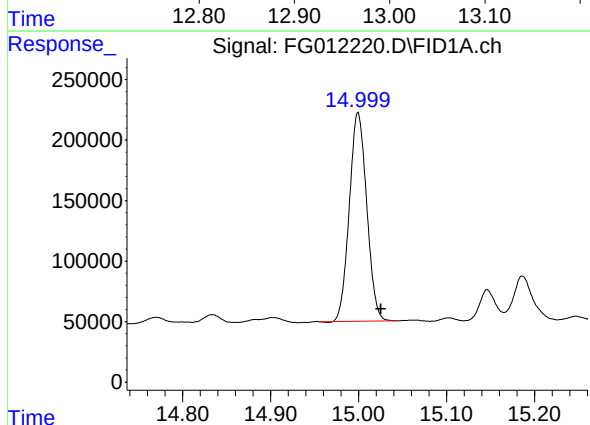


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.999 min
Delta R.T.: -0.026 min
Response: 2374786
Conc: 17.81 ug/ml

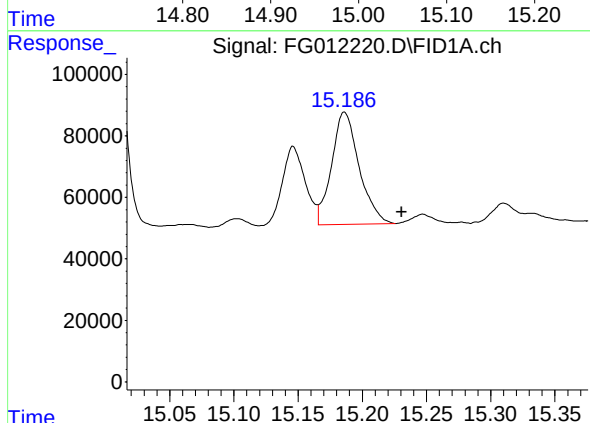


#10 N-TETRACOSANE

R.T.: 15.186 min
Delta R.T.: -0.044 min
Response: 545764
Conc: 3.65 ug/ml

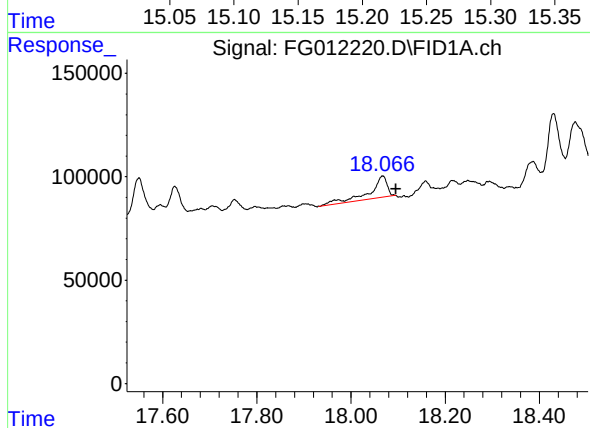

#13 N-TRIACONTANE

R.T.: 18.067 min
Delta R.T.: -0.028 min
Response: 265314
Conc: 2.00 ug/ml

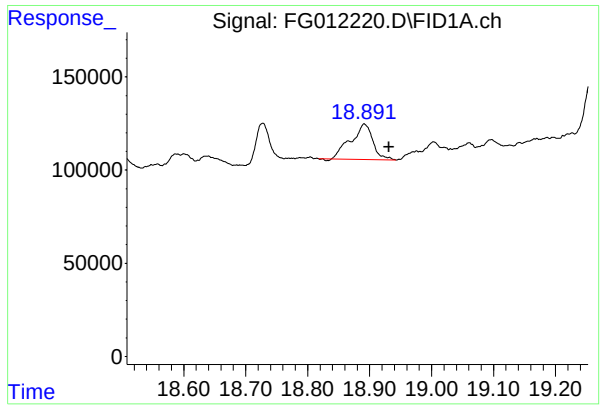

#14 N-DOTRIACONTANE

R.T.: 18.891 min
Delta R.T.: -0.039 min
Response: 470188
Conc: 3.68 ug/ml

Instrument :
FID_G
ClientSampleId :