

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061923\
 Data File : FG012223.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jun 2023 00:04
 Operator : YP\AJ
 Sample : 03308-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 04:29:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
 Quant Title :
 QLast Update : Thu Jun 01 17:30:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.040	480611	3.605 ug/ml
Target Compounds			
7) N-EICOSANE	12.964	970847	6.118 ug/ml
10) N-TETRACOSANE	15.187	799972	5.355 ug/ml
12) N-OCTACOSANE	17.197	311354	2.300 ug/ml
13) N-TRIACONTANE	18.066	383127	2.892 ug/ml
14) N-DOTRIACONTANE	18.893	527467	4.132 ug/ml
15) N-TETRATRIACONTANE	19.752	239037	1.964 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061923\
Data File : FG012223.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2023 00:04
Operator : YP\AJ
Sample : 03308-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 04:29:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

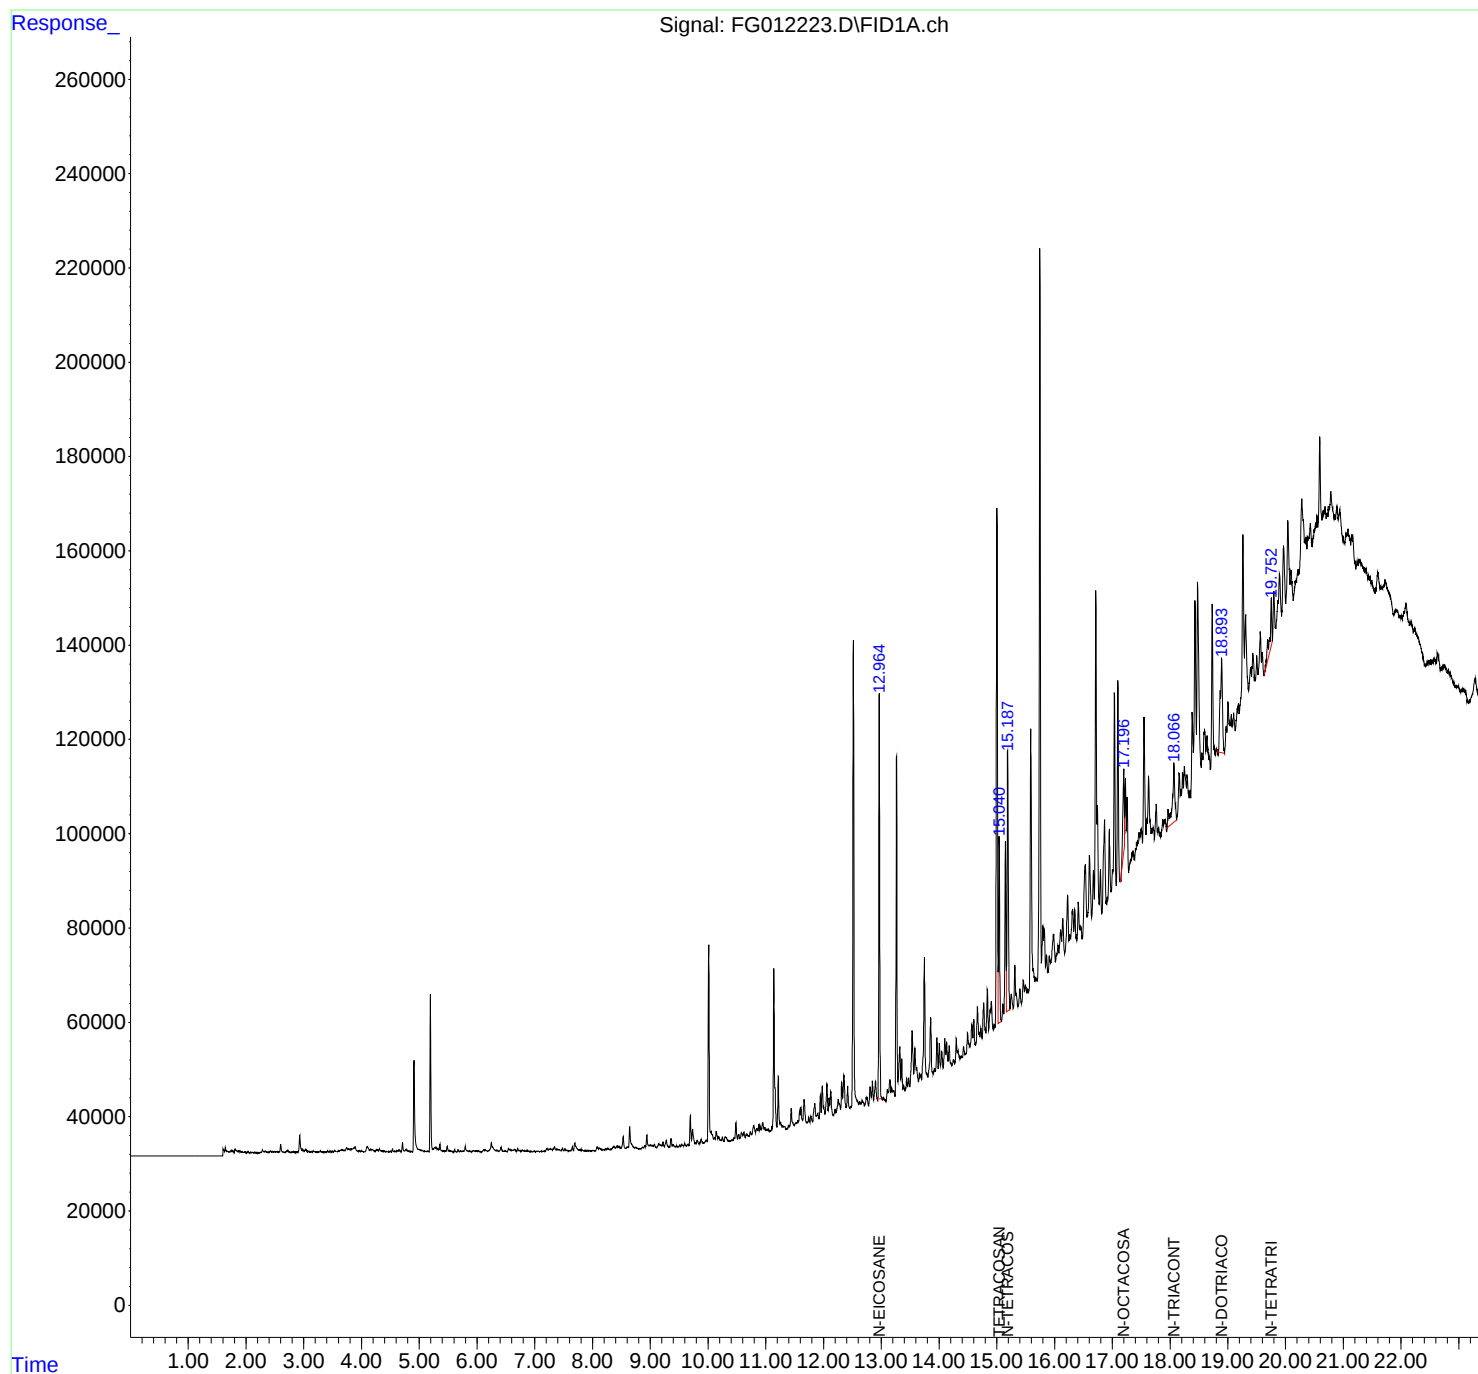


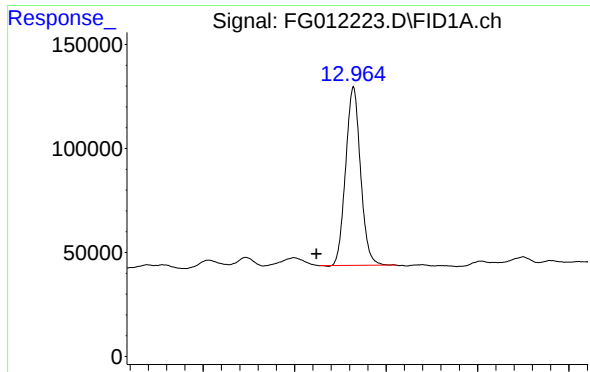

#7 N-EICOSANE


R.T.: 12.964 min
Delta R.T.: 0.040 min
Response: 970847
Conc: 6.12 ug/ml

Instrument :
FID_G
ClientSampleId :

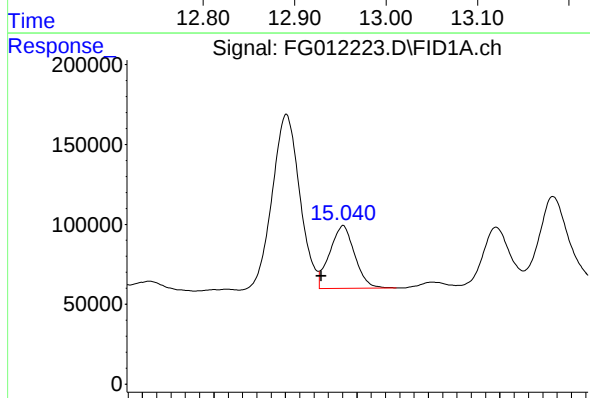


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.040 min
Delta R.T.: 0.015 min
Response: 480611
Conc: 3.60 ug/ml

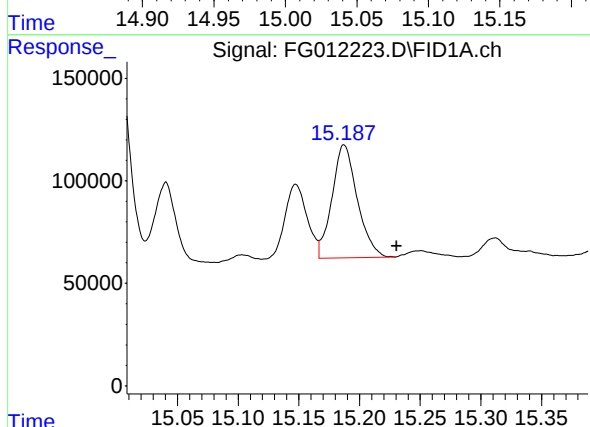


#10 N-TETRACOSANE

R.T.: 15.187 min
Delta R.T.: -0.043 min
Response: 799972
Conc: 5.36 ug/ml

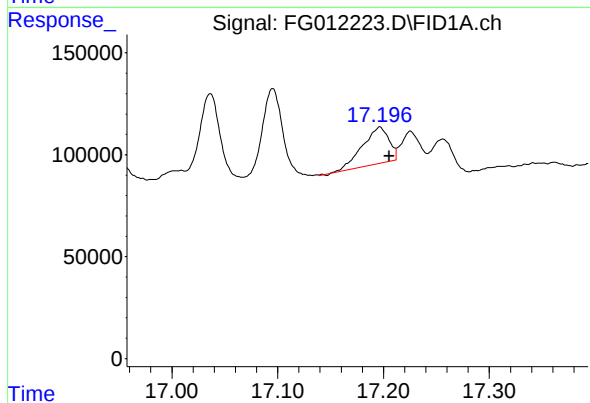

#12 N-OCTACOSANE


R.T.: 17.197 min
Delta R.T.: -0.009 min
Response: 311354
Conc: 2.30 ug/ml

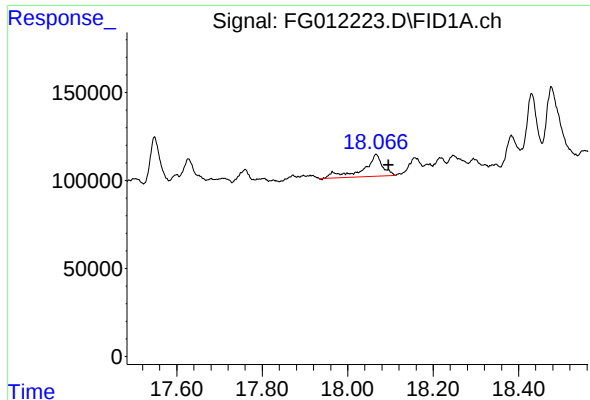

#13 N-TRIACONTANE


R.T.: 18.066 min
Delta R.T.: -0.029 min
Response: 383127
Conc: 2.89 ug/ml

Instrument :
FID_G
ClientSampleId :

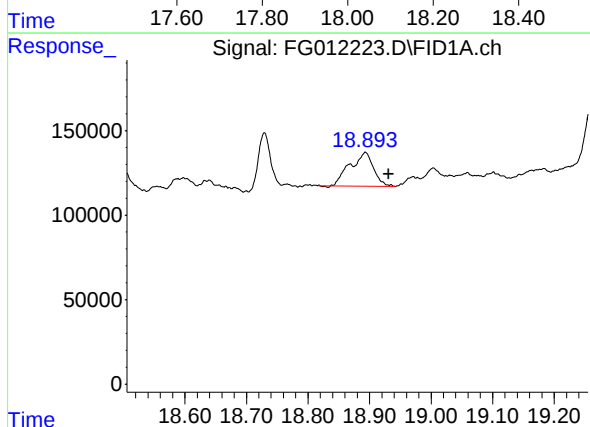

#14 N-DOTRIACONTANE

R.T.: 18.893 min
Delta R.T.: -0.038 min
Response: 527467
Conc: 4.13 ug/ml

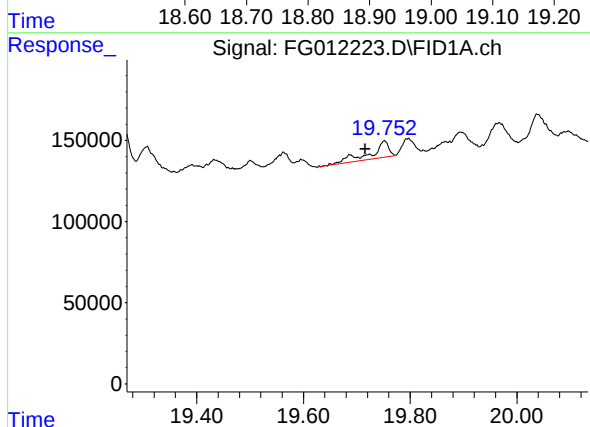

#15 N-TETRATRIACONTANE

R.T.: 19.752 min
Delta R.T.: 0.036 min
Response: 239037
Conc: 1.96 ug/ml