

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061923\
 Data File : FG012229.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jun 2023 04:28
 Operator : YP\AJ
 Sample : 03308-22
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 06:03:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
 Quant Title :
 QLast Update : Thu Jun 01 17:30:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.999	1682632	12.620 ug/ml
Target Compounds			
7) N-EICOSANE	12.963	984576	6.204 ug/ml
10) N-TETRACOSANE	15.184	1388766	9.297 ug/ml
11) N-HEXACOSANE	16.225	221306	1.563 ug/ml
12) N-OCTACOSANE	17.194	501684	3.706 ug/ml
13) N-TRIACONTANE	18.065	462273	3.489 ug/ml
14) N-DOTRIACONTANE	18.892	551694	4.322 ug/ml
15) N-TETRATRIACONTANE	19.684	191032	1.569 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG061923\
Data File : FG012229.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2023 04:28
Operator : YP\AJ
Sample : 03308-22
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 06:03:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

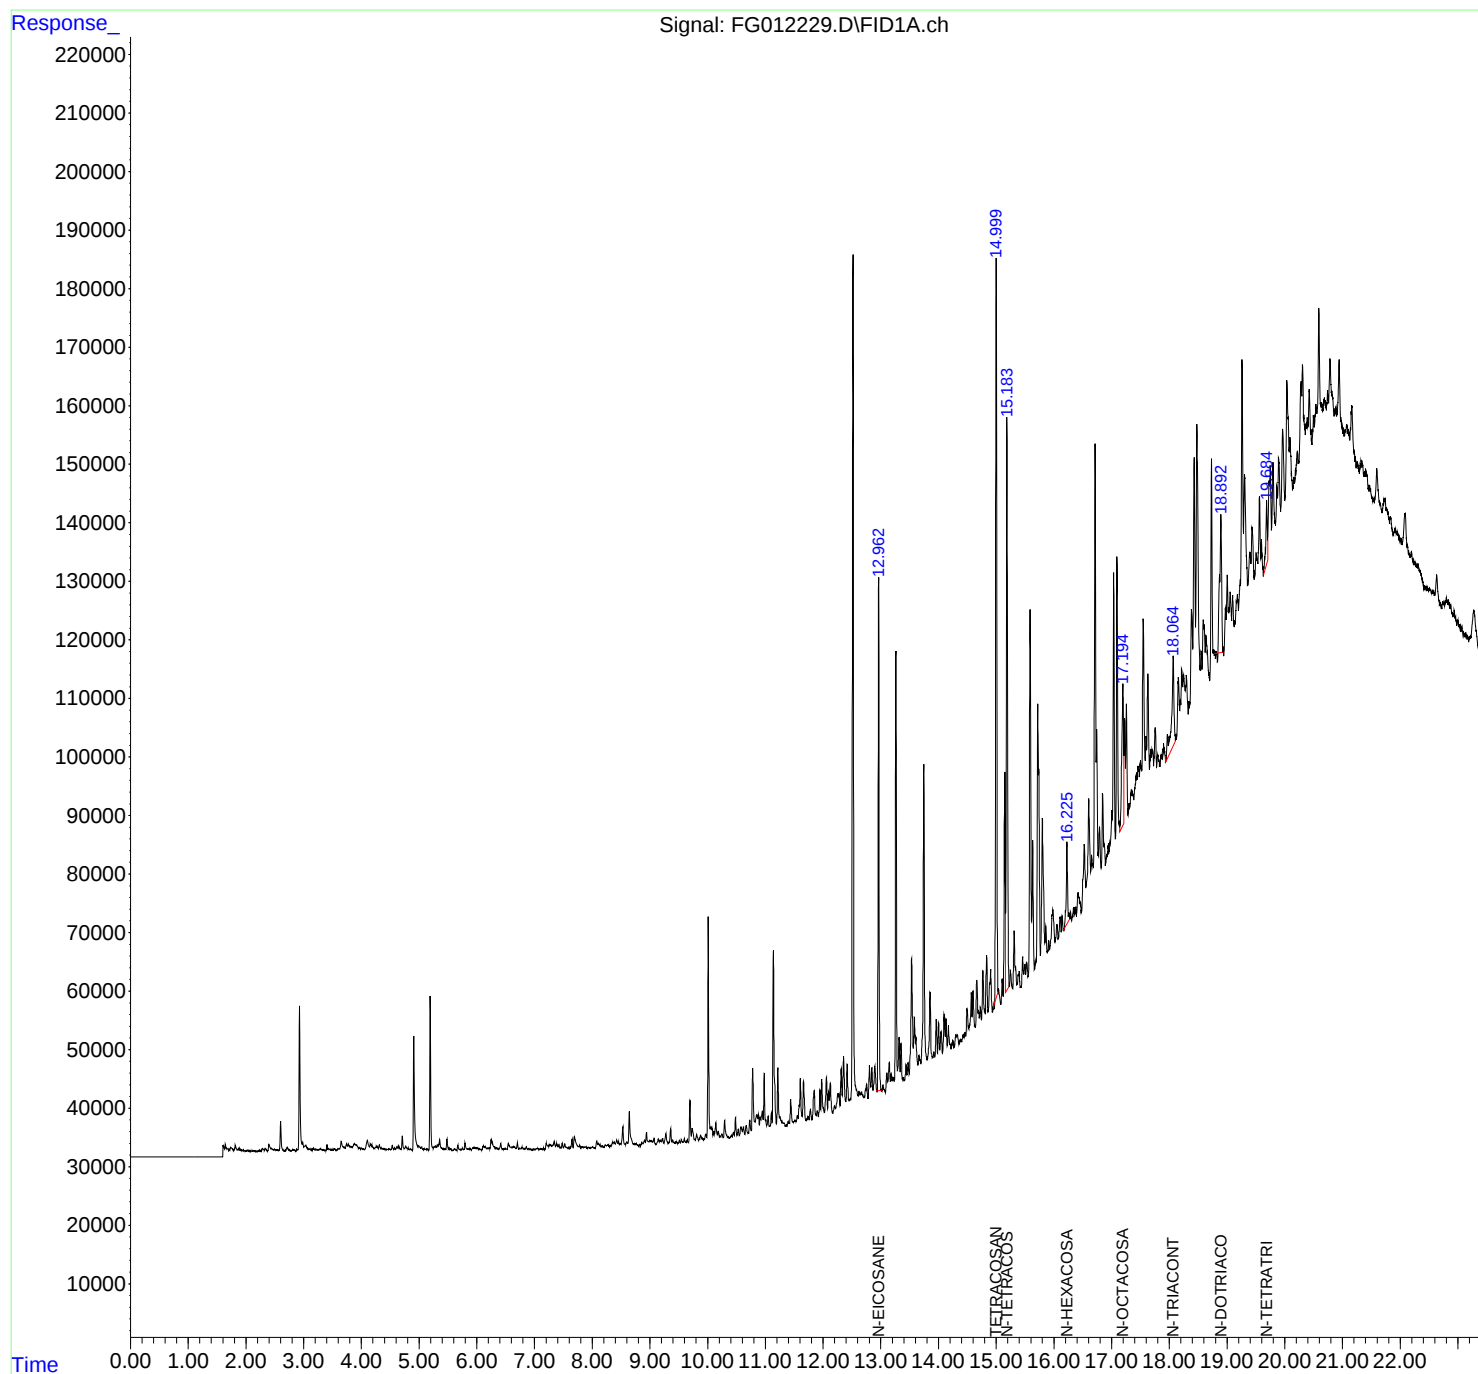


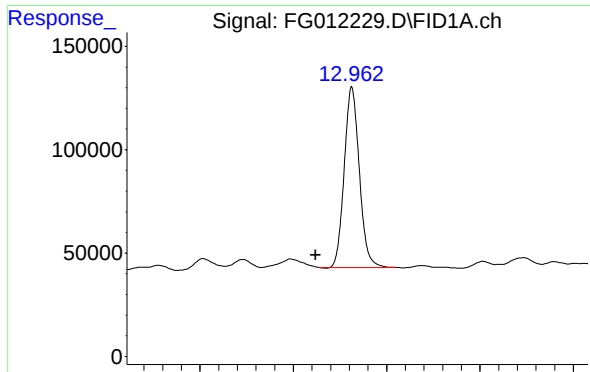

#7 N-EICOSANE


R.T.: 12.963 min
Delta R.T.: 0.039 min
Response: 984576
Conc: 6.20 ug/ml

Instrument :
FID_G
ClientSampleId :

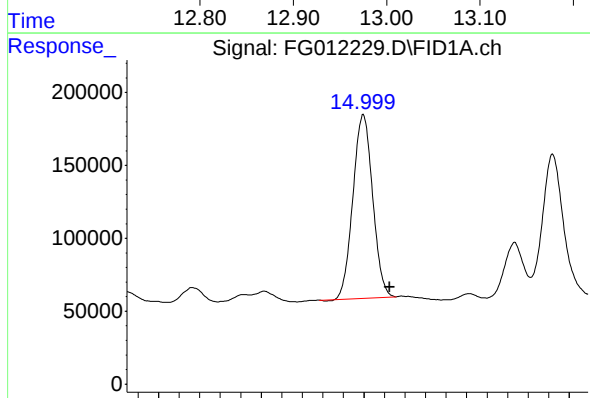


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.999 min
Delta R.T.: -0.026 min
Response: 1682632
Conc: 12.62 ug/ml

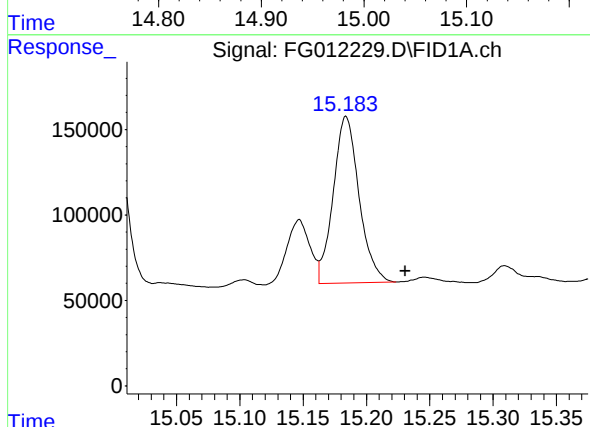


#10 N-TETRACOSANE

R.T.: 15.184 min
Delta R.T.: -0.047 min
Response: 1388766
Conc: 9.30 ug/ml

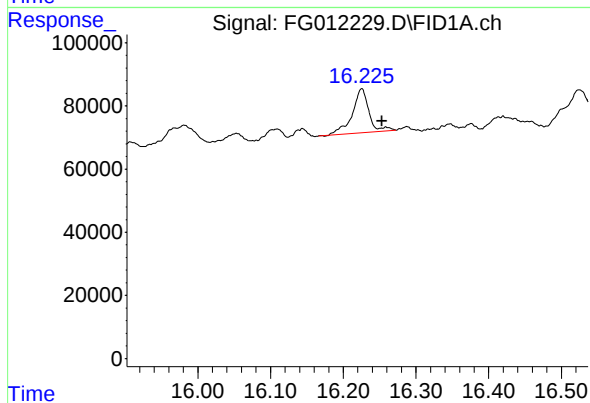

#11 N-HEXACOSANE


R.T.: 16.225 min
Delta R.T.: -0.028 min
Response: 221306
Conc: 1.56 ug/ml

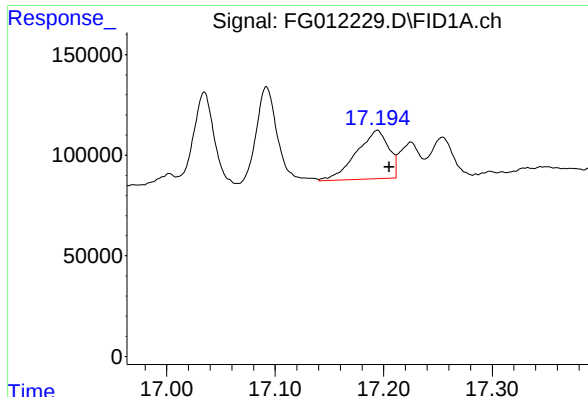

#12 N-OCTACOSANE


R.T.: 17.194 min
Delta R.T.: -0.011 min
Response: 501684
Conc: 3.71 ug/ml

Instrument :
FID_G
ClientSampleId :

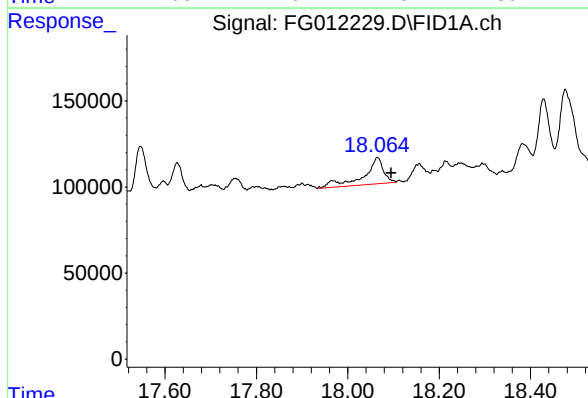


#13 N-TRIACONTANE

R.T.: 18.065 min
Delta R.T.: -0.031 min
Response: 462273
Conc: 3.49 ug/ml

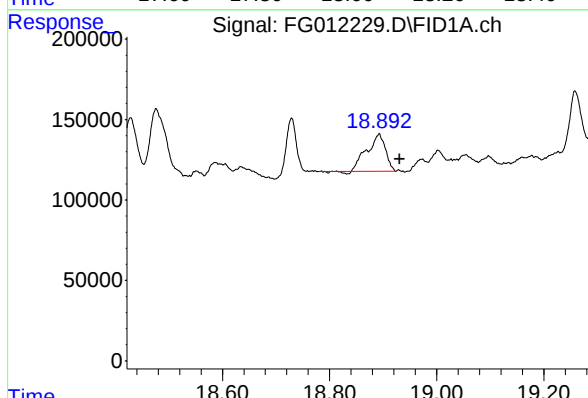

#14 N-DOTRIACONTANE

R.T.: 18.892 min
Delta R.T.: -0.038 min
Response: 551694
Conc: 4.32 ug/ml

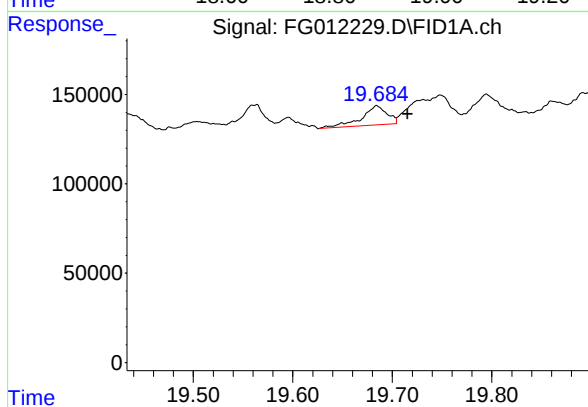

#15 N-TETRATRIACONTANE

R.T.: 19.684 min
Delta R.T.: -0.031 min
Response: 191032
Conc: 1.57 ug/ml