

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
Data File : FG001396.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2018 10:41
Operator : UA\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:56:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.291	4578758	33.029 ug/ml
12)	N-OCTACOSANE	16.712	4552160	32.992 ug/ml
13)	N-TRIACONTANE	17.597	452185	3.296 ug/ml
14)	N-DOTRIACONTANE	18.433	670103	5.010 ug/ml
15)	N-TETRATRIACONTANE	19.220	484618	3.679 ug/ml
16)	N-HEXATRIACONTANE	19.964	282224	2.246 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
Data File : FG001396.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2018 10:41
Operator : UA\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:56:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

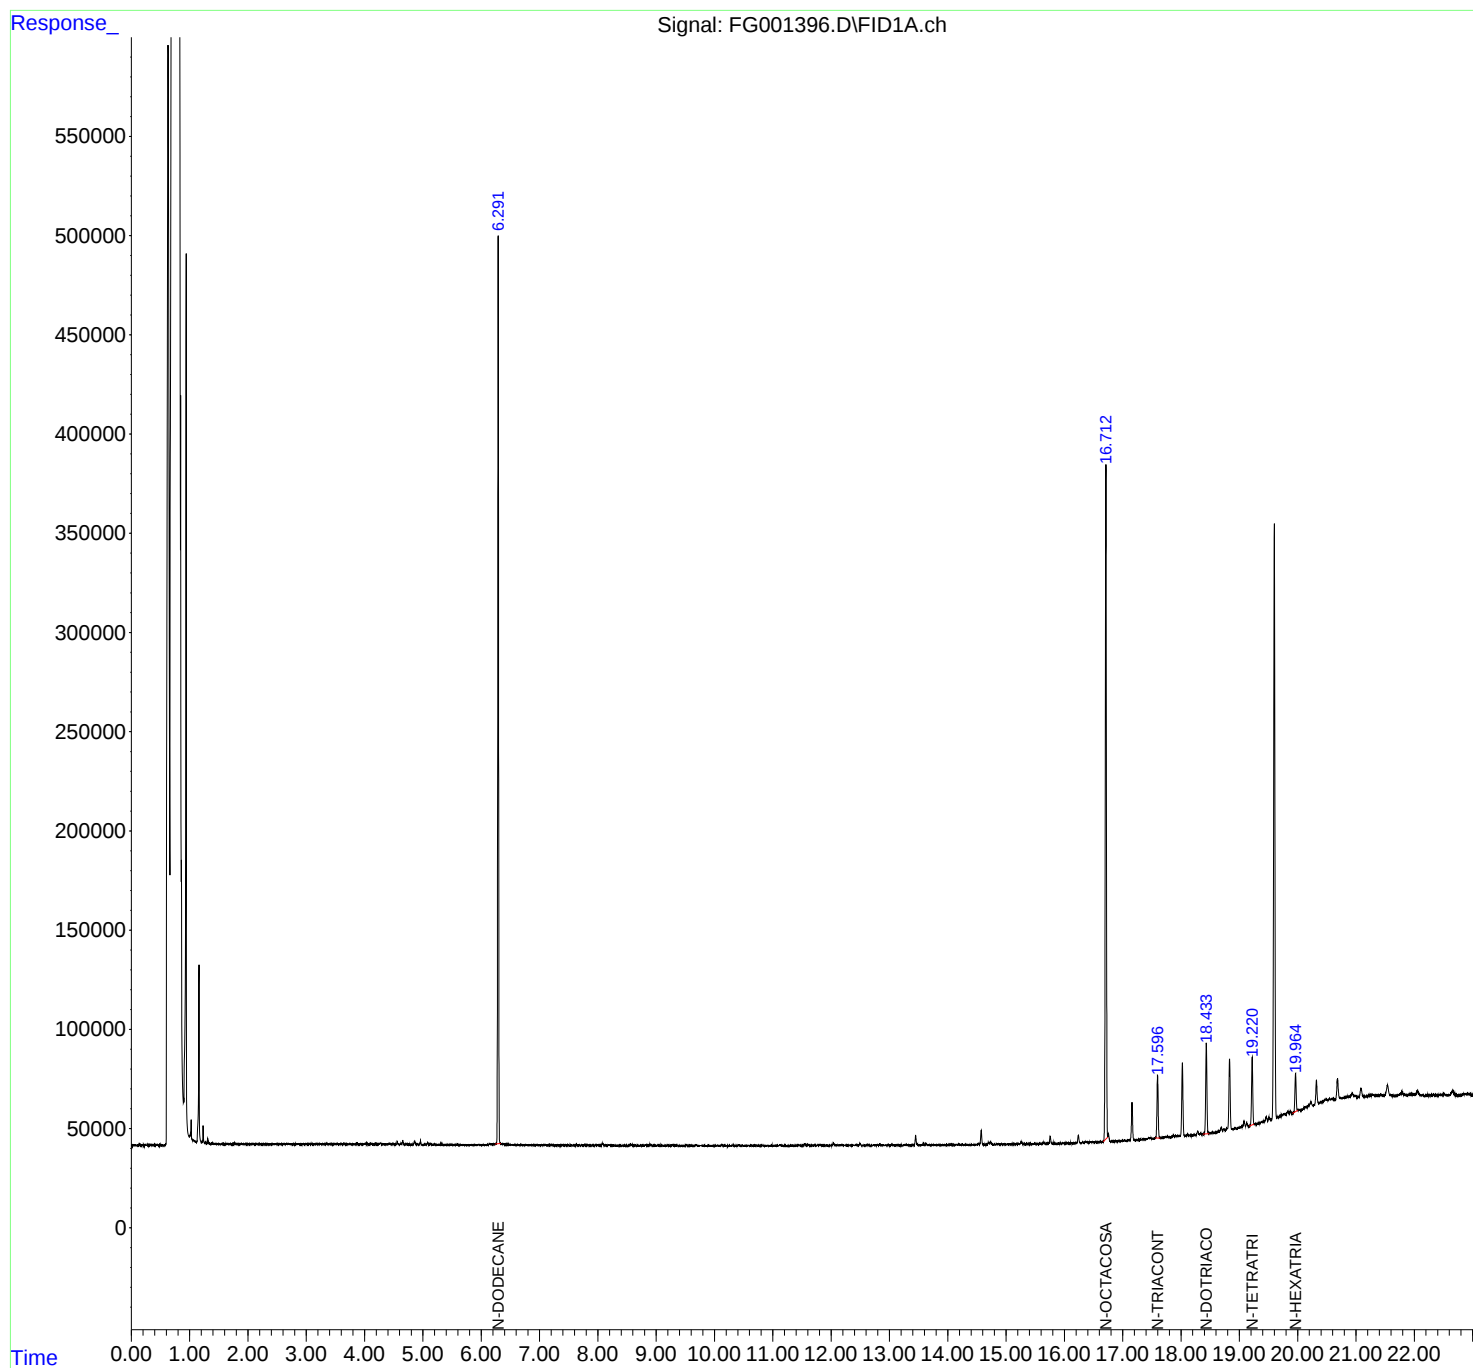


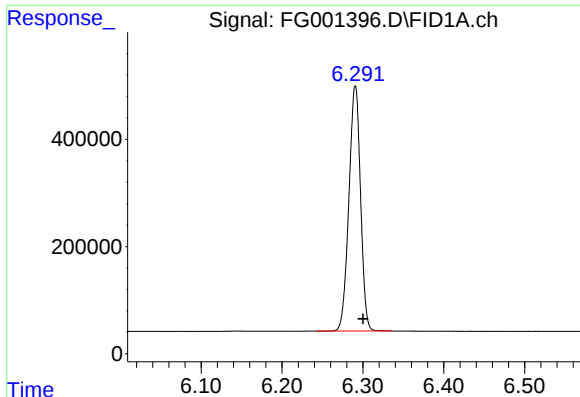

#3 N-DODECANE


R.T.: 6.291 min
Delta R.T.: -0.010 min
Response: 4578758
Conc: 33.03 ug/ml

Instrument :
FID_G
ClientSampleId :

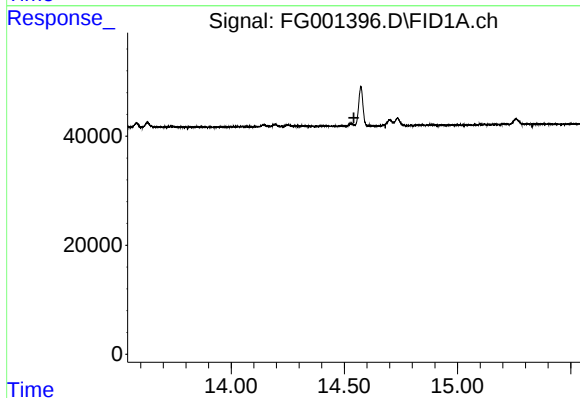


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.542 min
Response: 0
Conc: N.D.

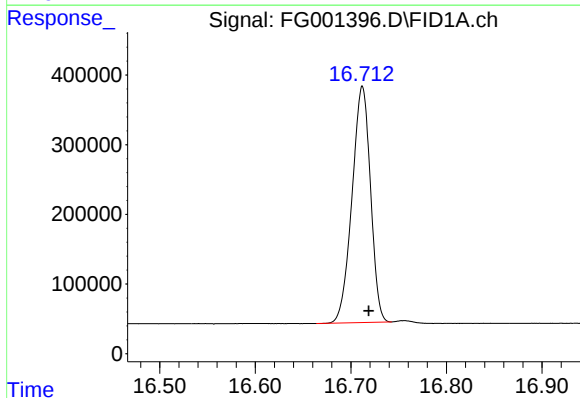


#12 N-OCTACOSANE

R.T.: 16.712 min
Delta R.T.: -0.007 min
Response: 4552160
Conc: 32.99 ug/ml

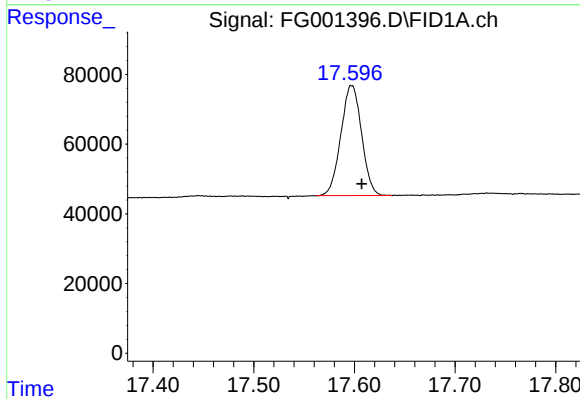

#13 N-TRIACONTANE


R.T.: 17.597 min
Delta R.T.: -0.010 min
Response: 452185
Conc: 3.30 ug/ml

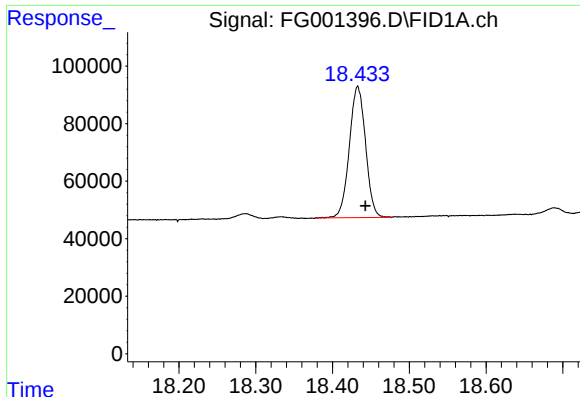

#14 N-DOTRIACONTANE


R.T.: 18.433 min
Delta R.T.: -0.010 min
Response: 670103
Conc: 5.01 ug/ml

Instrument :
FID_G
ClientSampleId :

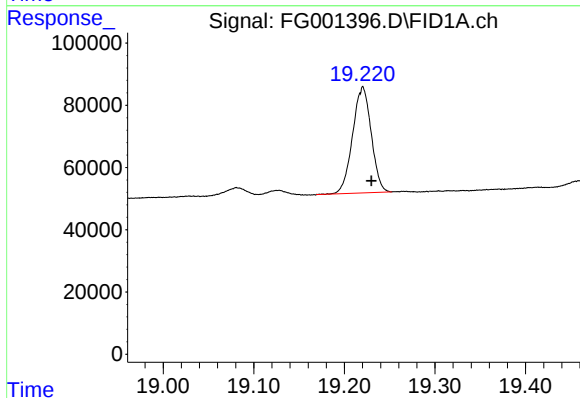

#15 N-TETRATRIACONTANE

R.T.: 19.220 min
Delta R.T.: -0.009 min
Response: 484618
Conc: 3.68 ug/ml

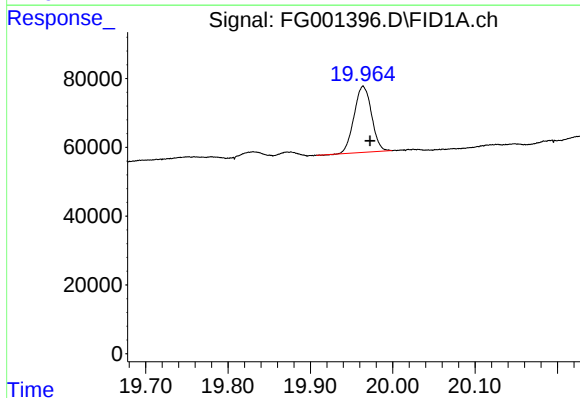

#16 N-HEXATRIACONTANE

R.T.: 19.964 min
Delta R.T.: -0.008 min
Response: 282224
Conc: 2.25 ug/ml