

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
 Data File : FG001408.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jun 2018 16:42
 Operator : UA\AJ
 Sample : J3584-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:59:19 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.533	2249675	18.402 ug/ml
Target Compounds			
4) N-TETRADECANE	8.136	456269	3.265 ug/ml
5) N-HEXADECANE	9.680	157139	1.117 ug/ml
12) N-OCTACOSANE	16.715	279915	2.029 ug/ml
13) N-TRIACONTANE	17.594	376041	2.741 ug/ml
14) N-DOTRIACONTANE	18.435	255256	1.908 ug/ml
15) N-TETRATRIACONTANE	19.239	311299	2.363 ug/ml
16) N-HEXATRIACONTANE	19.970	225307	1.793 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
Data File : FG001408.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2018 16:42
Operator : UA\AJ
Sample : J3584-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:59:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

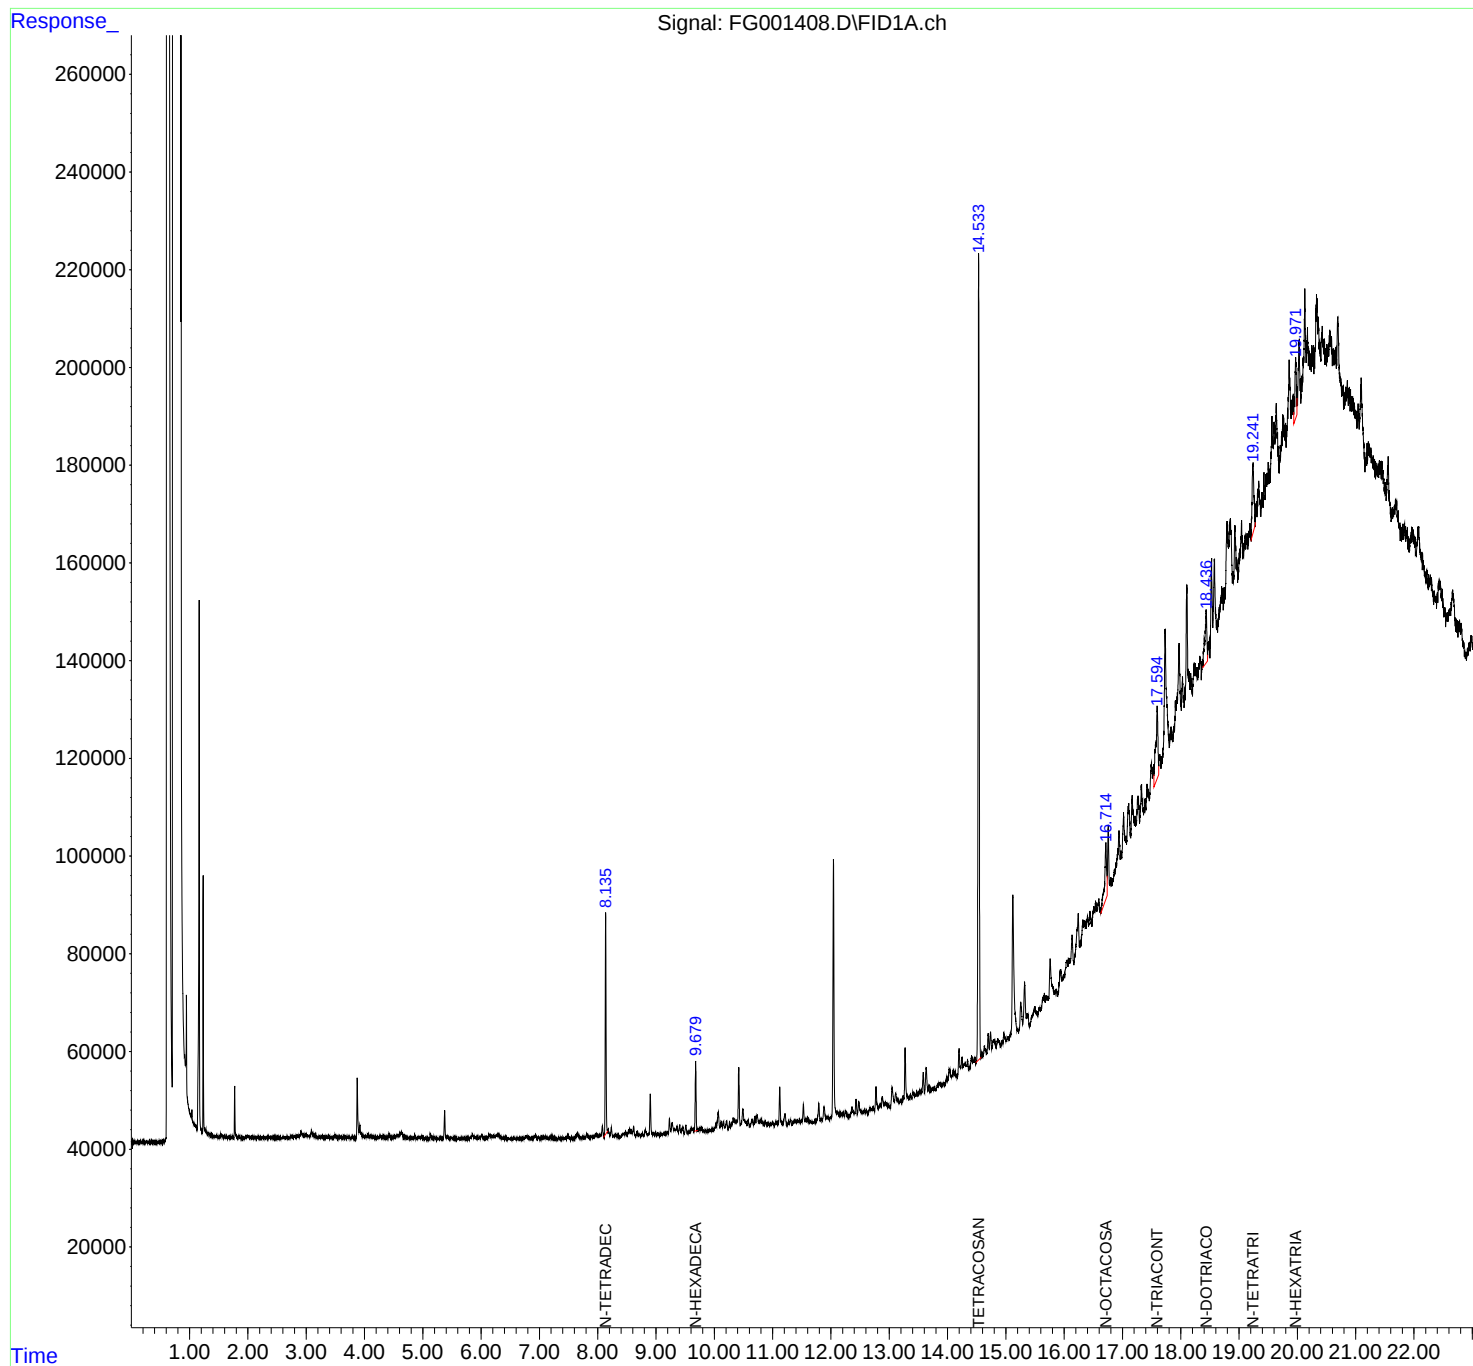


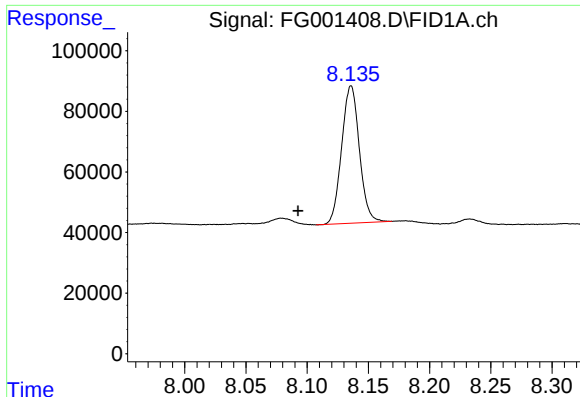

#4 N-TETRADECANE


R.T.: 8.136 min
Delta R.T.: 0.043 min
Response: 456269
Conc: 3.27 ug/ml

Instrument :
FID_G
ClientSampleId :

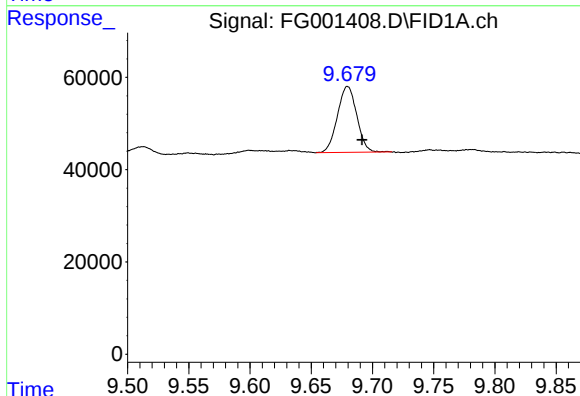


#5 N-HEXADECANE

R.T.: 9.680 min
Delta R.T.: -0.012 min
Response: 157139
Conc: 1.12 ug/ml

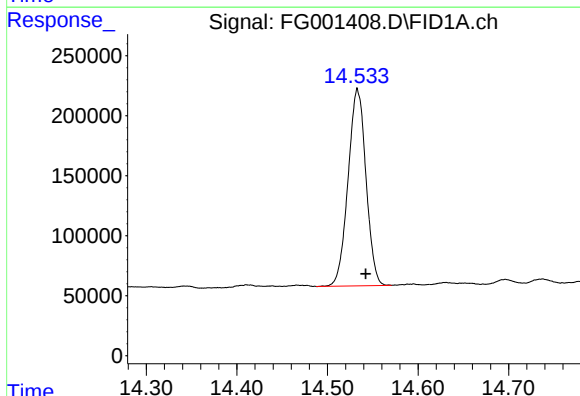


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.533 min
Delta R.T.: -0.009 min
Response: 2249675
Conc: 18.40 ug/ml

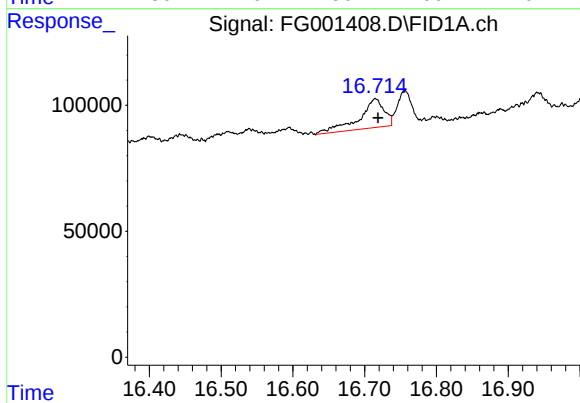

#12 N-OCTACOSANE


R.T.: 16.715 min
Delta R.T.: -0.004 min
Response: 279915
Conc: 2.03 ug/ml

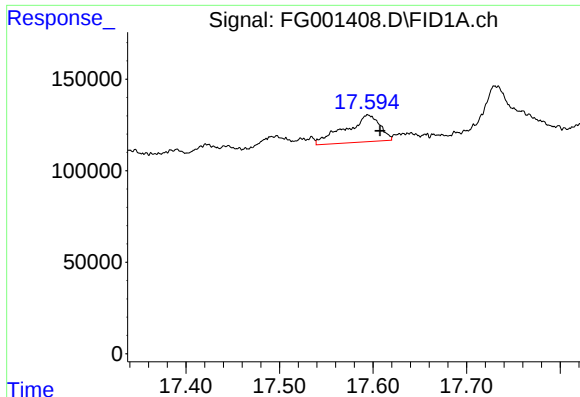

#13 N-TRIACONTANE


R.T.: 17.594 min
Delta R.T.: -0.013 min
Response: 376041
Conc: 2.74 ug/ml

Instrument :
FID_G
ClientSampleId :

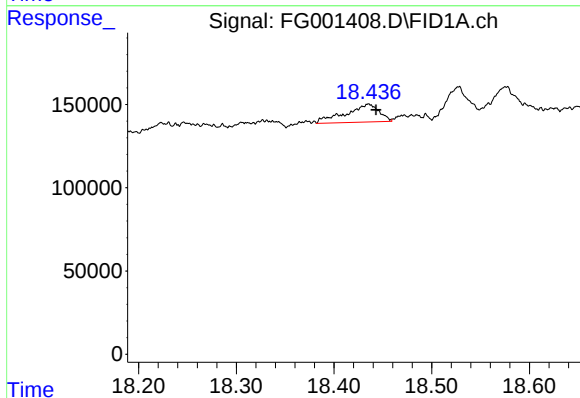


#14 N-DOTRIACONTANE

R.T.: 18.435 min
Delta R.T.: -0.008 min
Response: 255256
Conc: 1.91 ug/ml

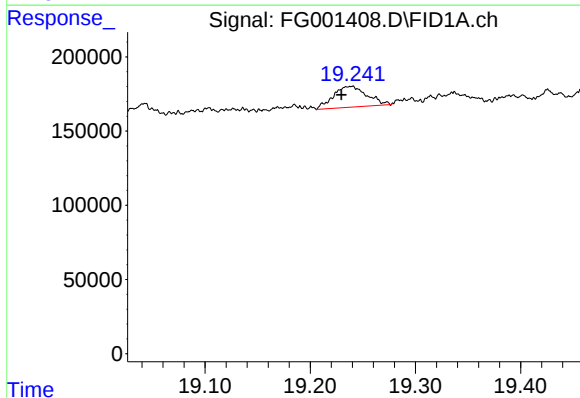

#15 N-TETRATRIACONTANE

R.T.: 19.239 min
Delta R.T.: 0.009 min
Response: 311299
Conc: 2.36 ug/ml

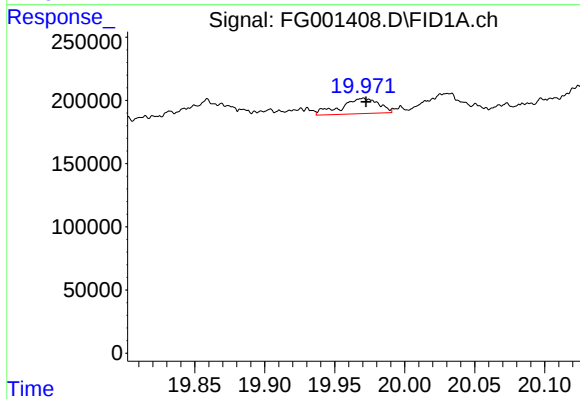

#16 N-HEXATRIACONTANE

R.T.: 19.970 min
Delta R.T.: -0.003 min
Response: 225307
Conc: 1.79 ug/ml