

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
 Data File : FG001411.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jun 2018 18:14
 Operator : UA\AJ
 Sample : J3584-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:59:57 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.534	1547542	12.659 ug/ml
Target Compounds			
4) N-TETRADECANE	8.136	473712	3.390 ug/ml
5) N-HEXADECANE	9.680	214350	1.523 ug/ml
7) N-EICOSANE	12.478	890843	6.326 ug/ml
10) N-TETRACOSANE	14.697	431869	3.106 ug/ml
12) N-OCTACOSANE	16.710	303511	2.200 ug/ml
13) N-TRIACONTANE	17.599	333516	2.431 ug/ml
14) N-DOTRIACONTANE	18.435	296067	2.214 ug/ml
15) N-TETRATRIACONTANE	19.230	194045	1.473 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
Data File : FG001411.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2018 18:14
Operator : UA\AJ
Sample : J3584-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:59:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

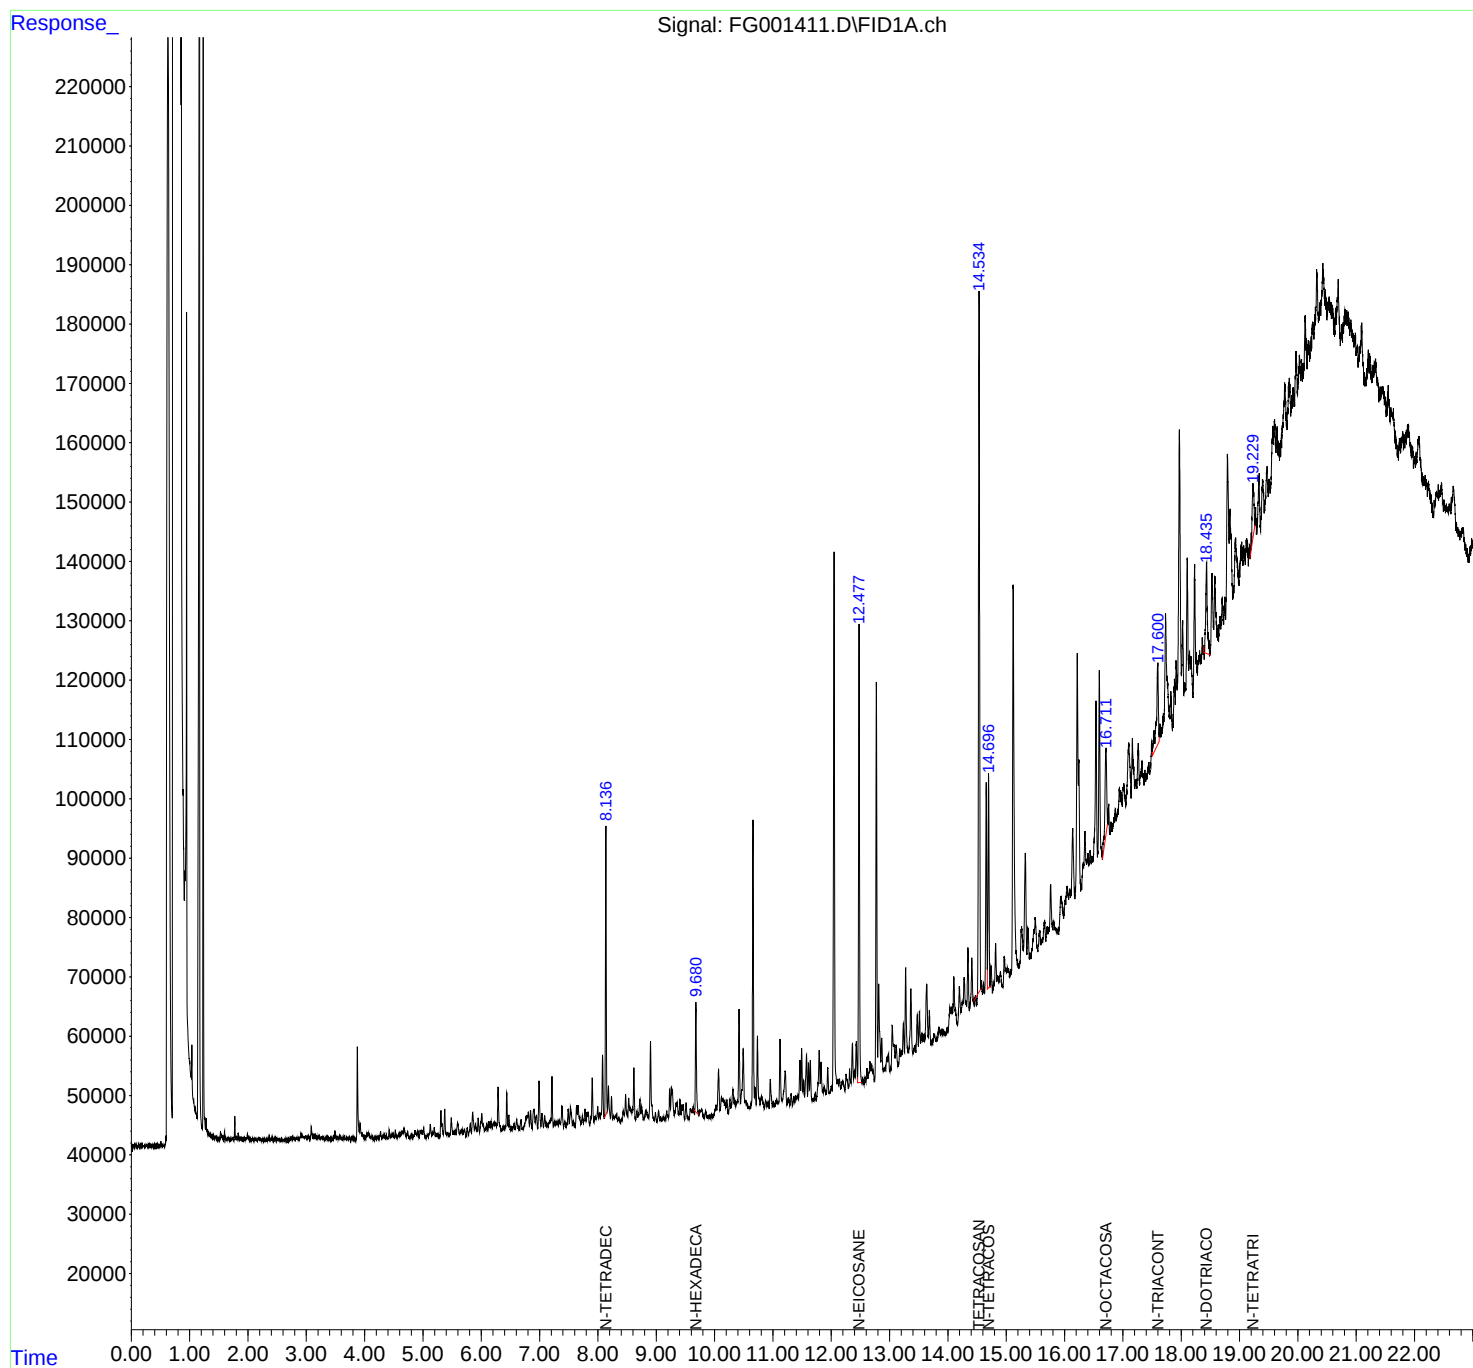


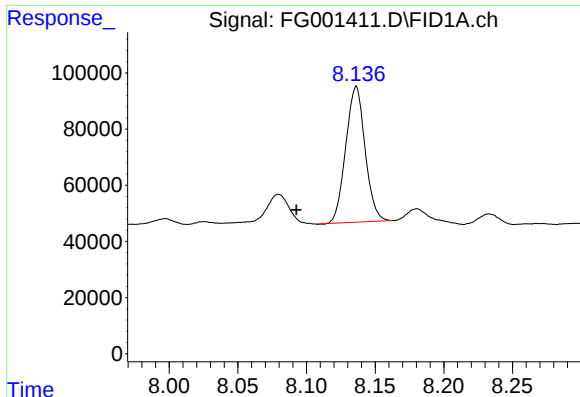

#4 N-TETRADECANE


R.T.: 8.136 min
Delta R.T.: 0.044 min
Response: 473712
Conc: 3.39 ug/ml

Instrument :
FID_G
ClientSampleId :

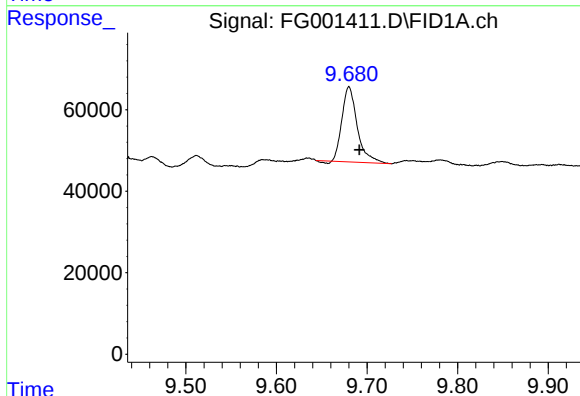


#5 N-HEXADECANE

R.T.: 9.680 min
Delta R.T.: -0.011 min
Response: 214350
Conc: 1.52 ug/ml

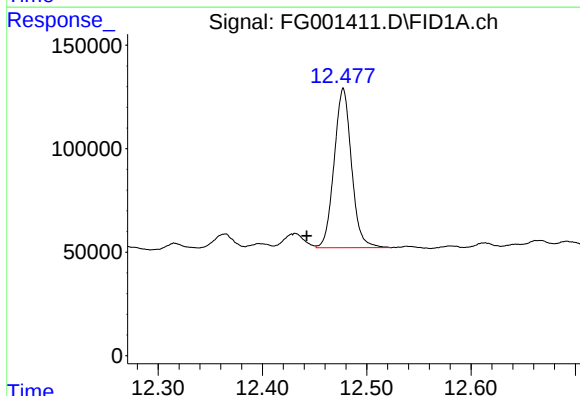


#7 N-EICOSANE

R.T.: 12.478 min
Delta R.T.: 0.035 min
Response: 890843
Conc: 6.33 ug/ml

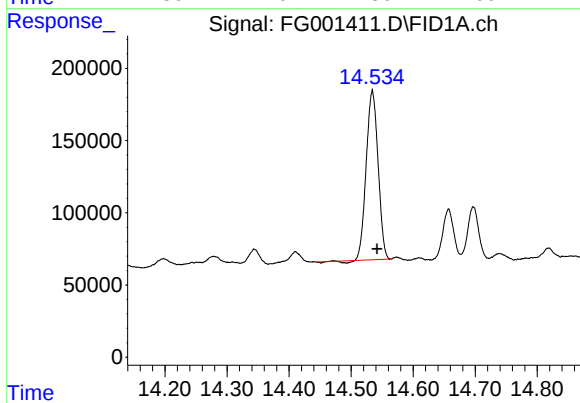

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.534 min
Delta R.T.: -0.008 min
Response: 1547542
Conc: 12.66 ug/ml

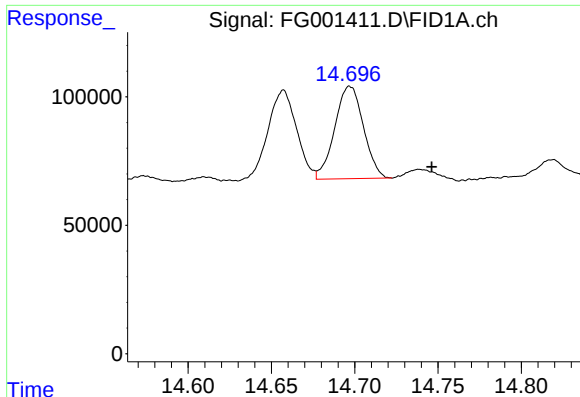

#10 N-TETRACOSANE


R.T.: 14.697 min
Delta R.T.: -0.049 min
Response: 431869
Conc: 3.11 ug/ml

Instrument :
FID_G
ClientSampleId :

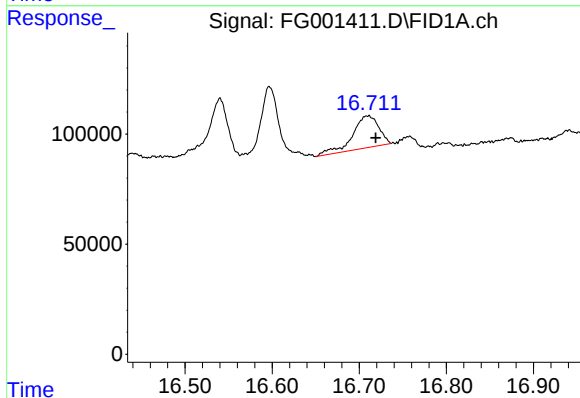


#12 N-OCTACOSANE

R.T.: 16.710 min
Delta R.T.: -0.009 min
Response: 303511
Conc: 2.20 ug/ml

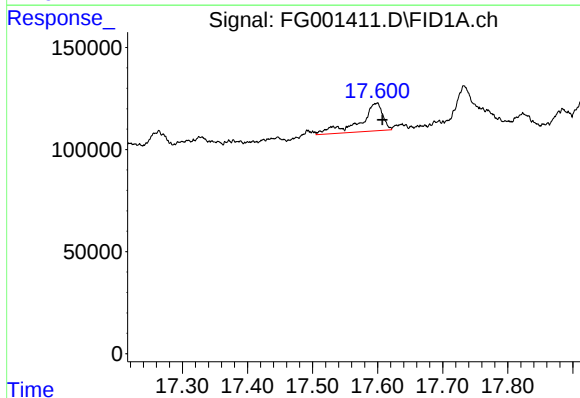


#13 N-TRIACONTANE

R.T.: 17.599 min
Delta R.T.: -0.008 min
Response: 333516
Conc: 2.43 ug/ml

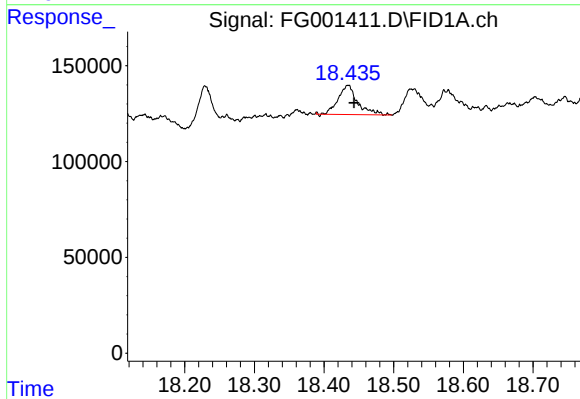

#14 N-DOTRIACONTANE

R.T.: 18.435 min
Delta R.T.: -0.008 min
Response: 296067
Conc: 2.21 ug/ml

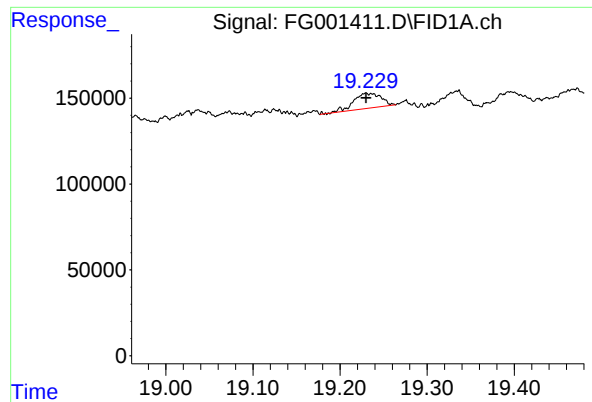

#15 N-TETRATRIACONTANE

R.T.: 19.230 min

Delta R.T.: 0.000 min

Response: 194045

Conc: 1.47 ug/ml

Instrument :
FID_G
ClientSampleId :