

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
 Data File : FG001412.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jun 2018 18:45
 Operator : UA\AJ
 Sample : J3584-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 08:00:12 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.535	2612537	21.370 ug/ml
Target Compounds			
4) N-TETRADECANE	8.137	503506	3.603 ug/ml
5) N-HEXADECANE	9.681	239046	1.699 ug/ml
6) N-OCTADECANE	11.123	159949	1.128 ug/ml
7) N-EICOSANE	12.478	840851	5.971 ug/ml
10) N-TETRACOSANE	14.698	424649	3.054 ug/ml
12) N-OCTACOSANE	16.707	249332	1.807 ug/ml
13) N-TRIACONTANE	17.598	318538	2.321 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
Data File : FG001412.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2018 18:45
Operator : UA\AJ
Sample : J3584-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 08:00:12 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

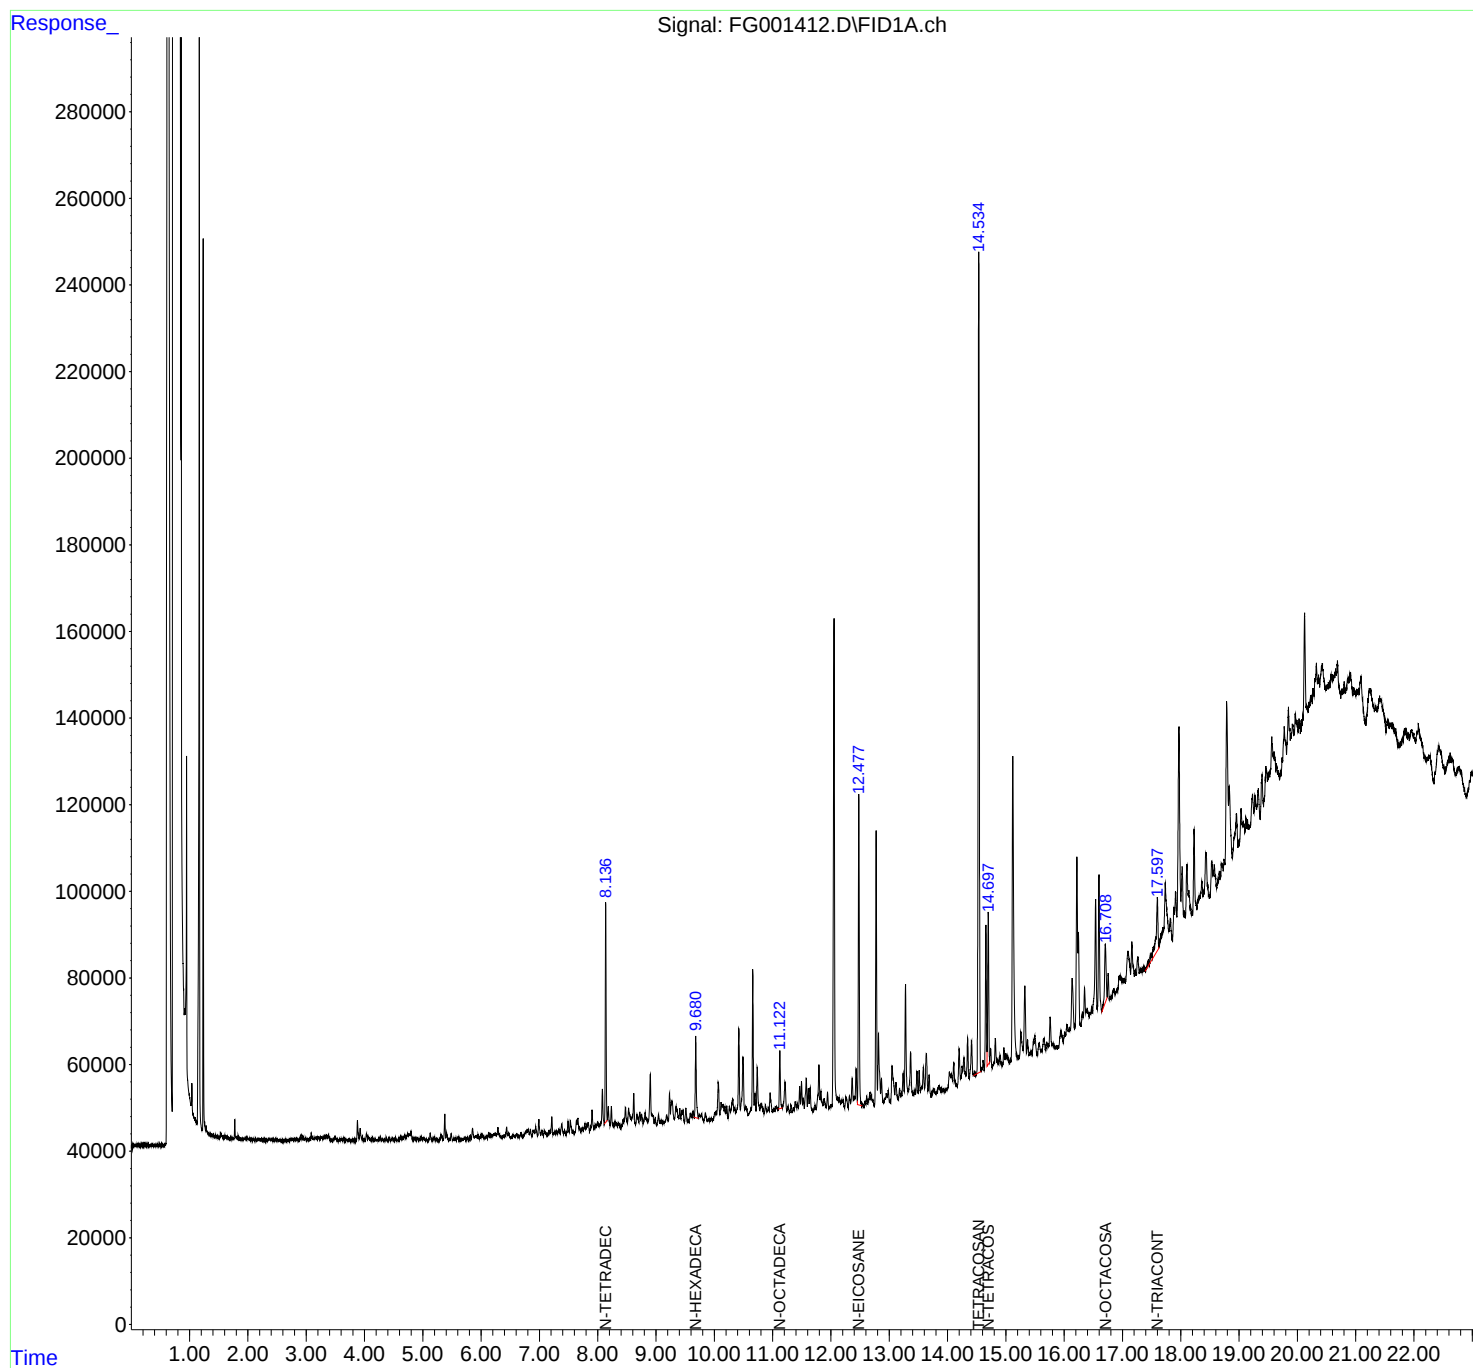


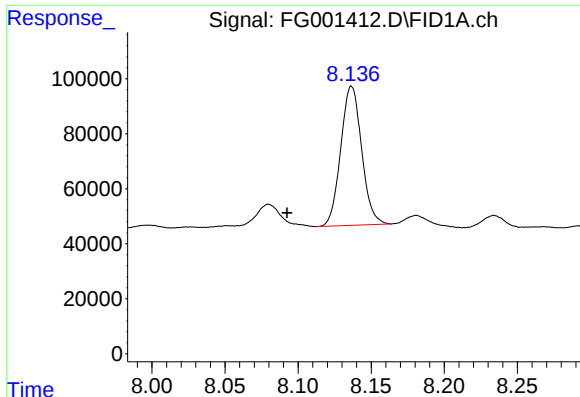

#4 N-TETRADECANE


R.T.: 8.137 min
Delta R.T.: 0.044 min
Response: 503506
Conc: 3.60 ug/ml

Instrument :
FID_G
ClientSampleId :

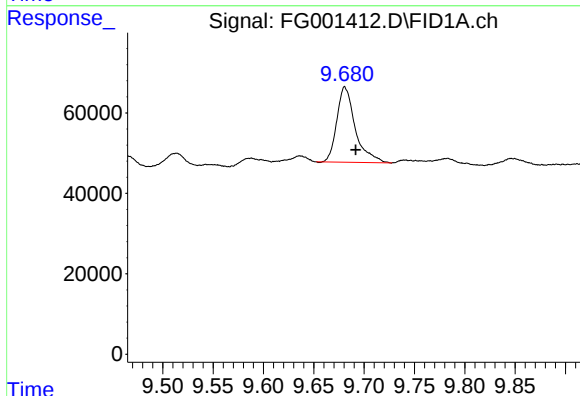


#5 N-HEXADECANE

R.T.: 9.681 min
Delta R.T.: -0.011 min
Response: 239046
Conc: 1.70 ug/ml

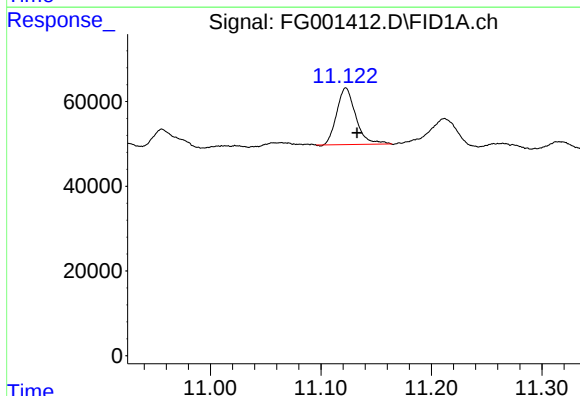


#6 N-OCTADECANE

R.T.: 11.123 min
Delta R.T.: -0.010 min
Response: 159949
Conc: 1.13 ug/ml

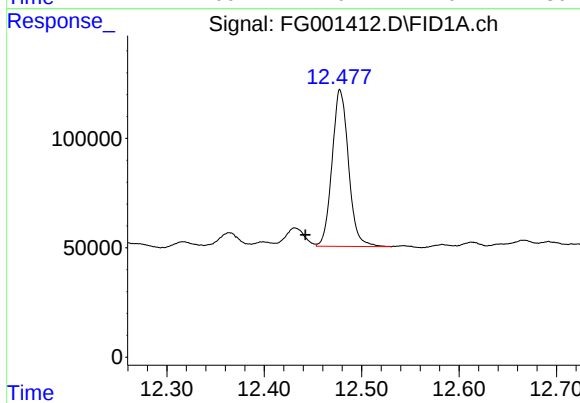

#7 N-EICOSANE


R.T.: 12.478 min
Delta R.T.: 0.035 min
Response: 840851
Conc: 5.97 ug/ml

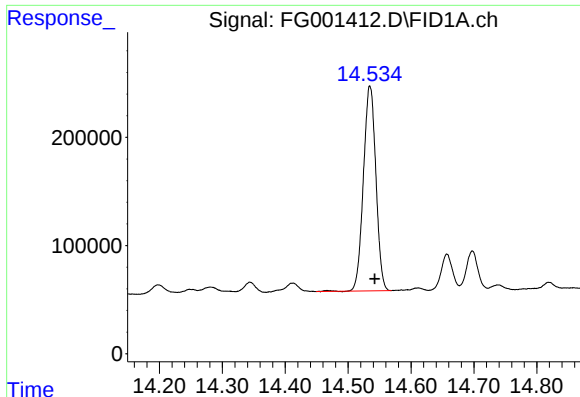

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.535 min
Delta R.T.: -0.008 min
Response: 2612537
Conc: 21.37 ug/ml

Instrument :
FID_G
ClientSampleId :

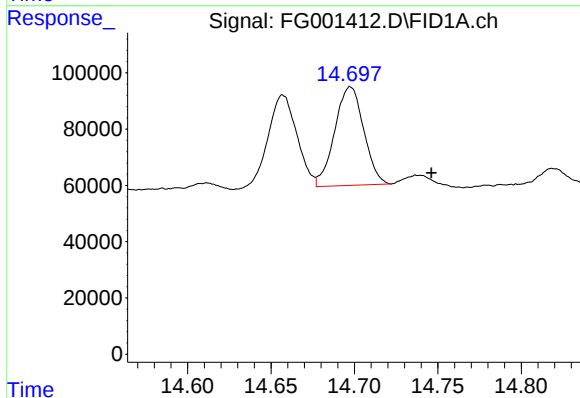


#10 N-TETRACOSANE

R.T.: 14.698 min
Delta R.T.: -0.049 min
Response: 424649
Conc: 3.05 ug/ml

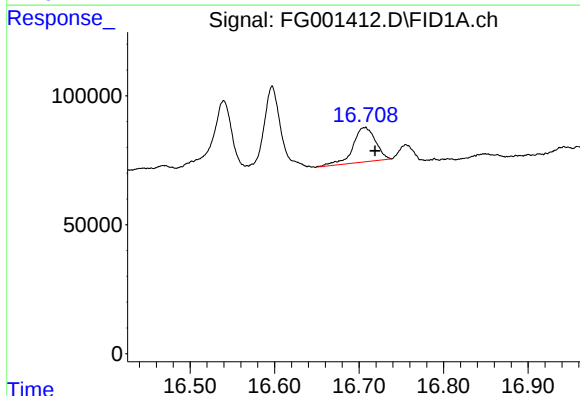

#12 N-OCTACOSANE

R.T.: 16.707 min
Delta R.T.: -0.012 min
Response: 249332
Conc: 1.81 ug/ml

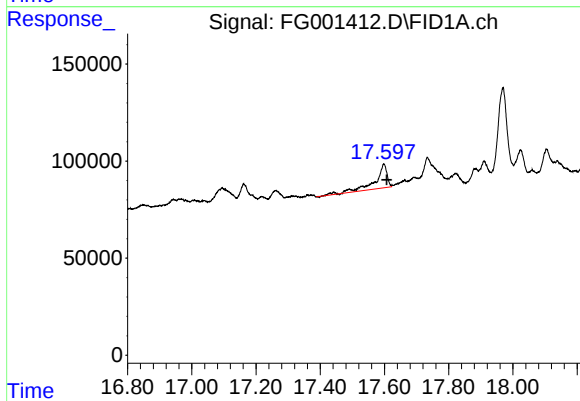

#13 N-TRIACONTANE

R.T.: 17.598 min
Delta R.T.: -0.009 min
Response: 318538
Conc: 2.32 ug/ml