

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
 Data File : FG001414.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jun 2018 19:46
 Operator : UA\AJ
 Sample : J3602-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 08:00:41 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.535	1785471	14.605 ug/ml
Target Compounds			
4) N-TETRADECANE	8.137	402460	2.880 ug/ml
6) N-OCTADECANE	11.125	258829	1.826 ug/ml
13) N-TRIACONTANE	17.596	162763	1.186 ug/ml
14) N-DOTRIACONTANE	18.432	379245	2.835 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
Data File : FG001414.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2018 19:46
Operator : UA\AJ
Sample : J3602-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 08:00:41 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

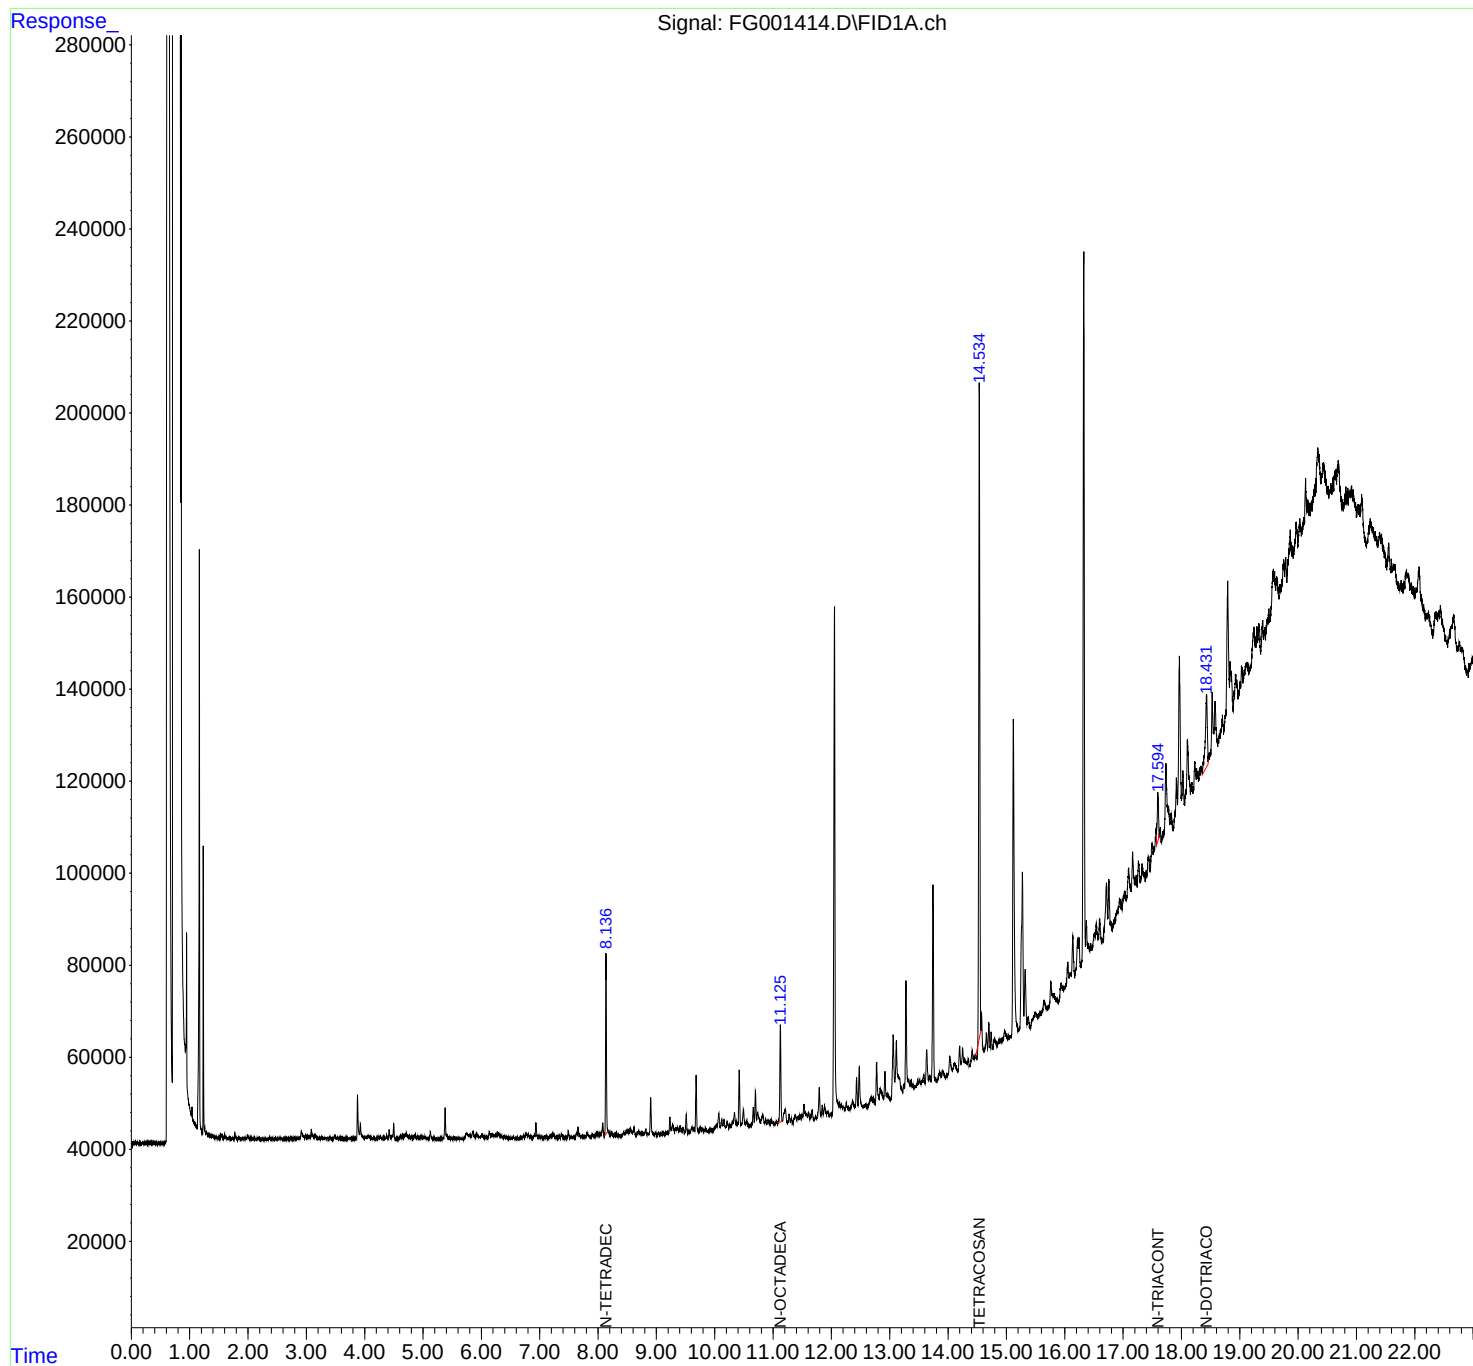


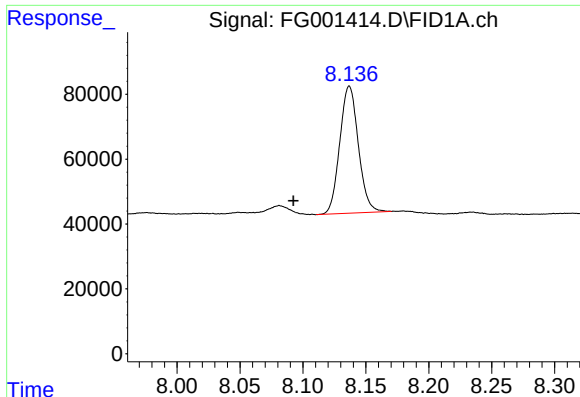

#4 N-TETRADECANE


R.T.: 8.137 min
Delta R.T.: 0.044 min
Response: 402460
Conc: 2.88 ug/ml

Instrument :
FID_G
ClientSampleId :

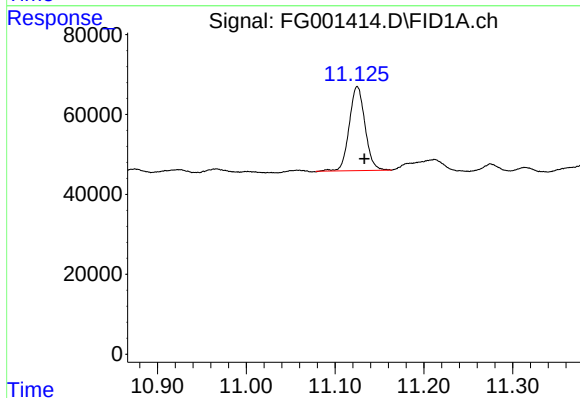


#6 N-OCTADECANE

R.T.: 11.125 min
Delta R.T.: -0.008 min
Response: 258829
Conc: 1.83 ug/ml

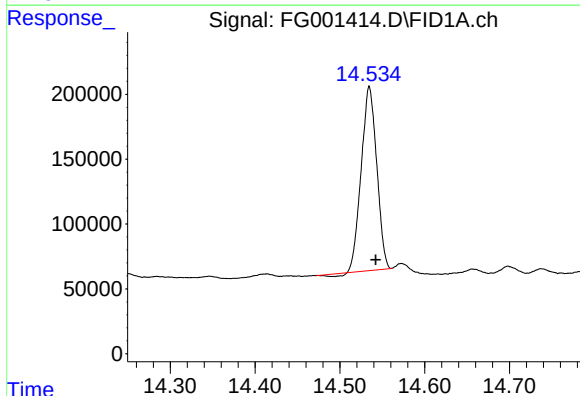


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.535 min
Delta R.T.: -0.008 min
Response: 1785471
Conc: 14.61 ug/ml

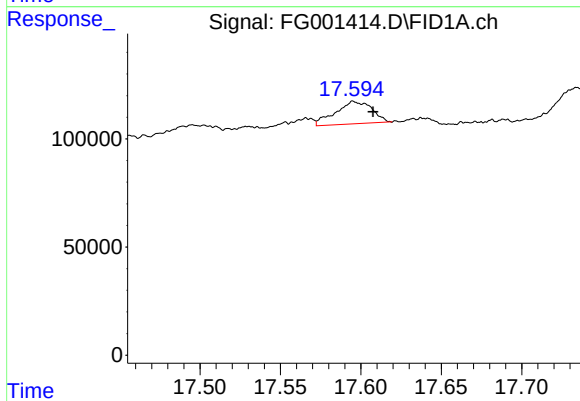

#13 N-TRIACONTANE

R.T.: 17.596 min
Delta R.T.: -0.012 min
Response: 162763
Conc: 1.19 ug/ml

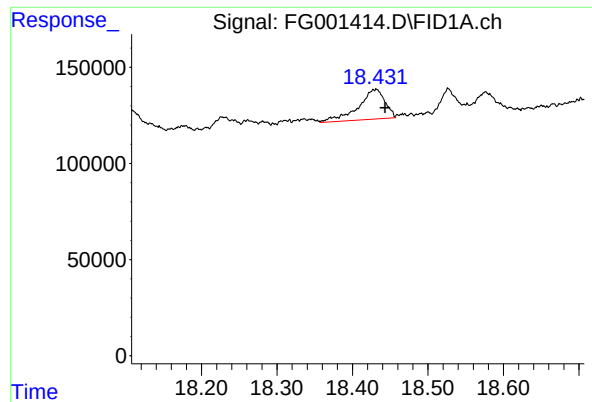

#14 N-DOTRIACONTANE

R.T.: 18.432 min
Delta R.T.: -0.011 min
Response: 379245
Conc: 2.84 ug/ml

Instrument :
FID_G
ClientSampleId :