

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
Data File : FG001414.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2018 19:46
Operator : UA\AJ
Sample : J3602-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Manual Integrations
APPROVED

UGO
6/21/2018 3:19:59 PM

Integration File: Sample.e
Quant Time: Jun 21 08:00:41 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.534	1939340	15.864 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062018\
Data File : FG001414.D
Signal(s) : FID1A.ch
Acq On : 20 Jun 2018 19:46
Operator : UA\AJ
Sample : J3602-02
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

UGO
6/21/2018 3:19:59 PM

Integration File: Sample.e
Quant Time: Jun 21 08:00:41 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

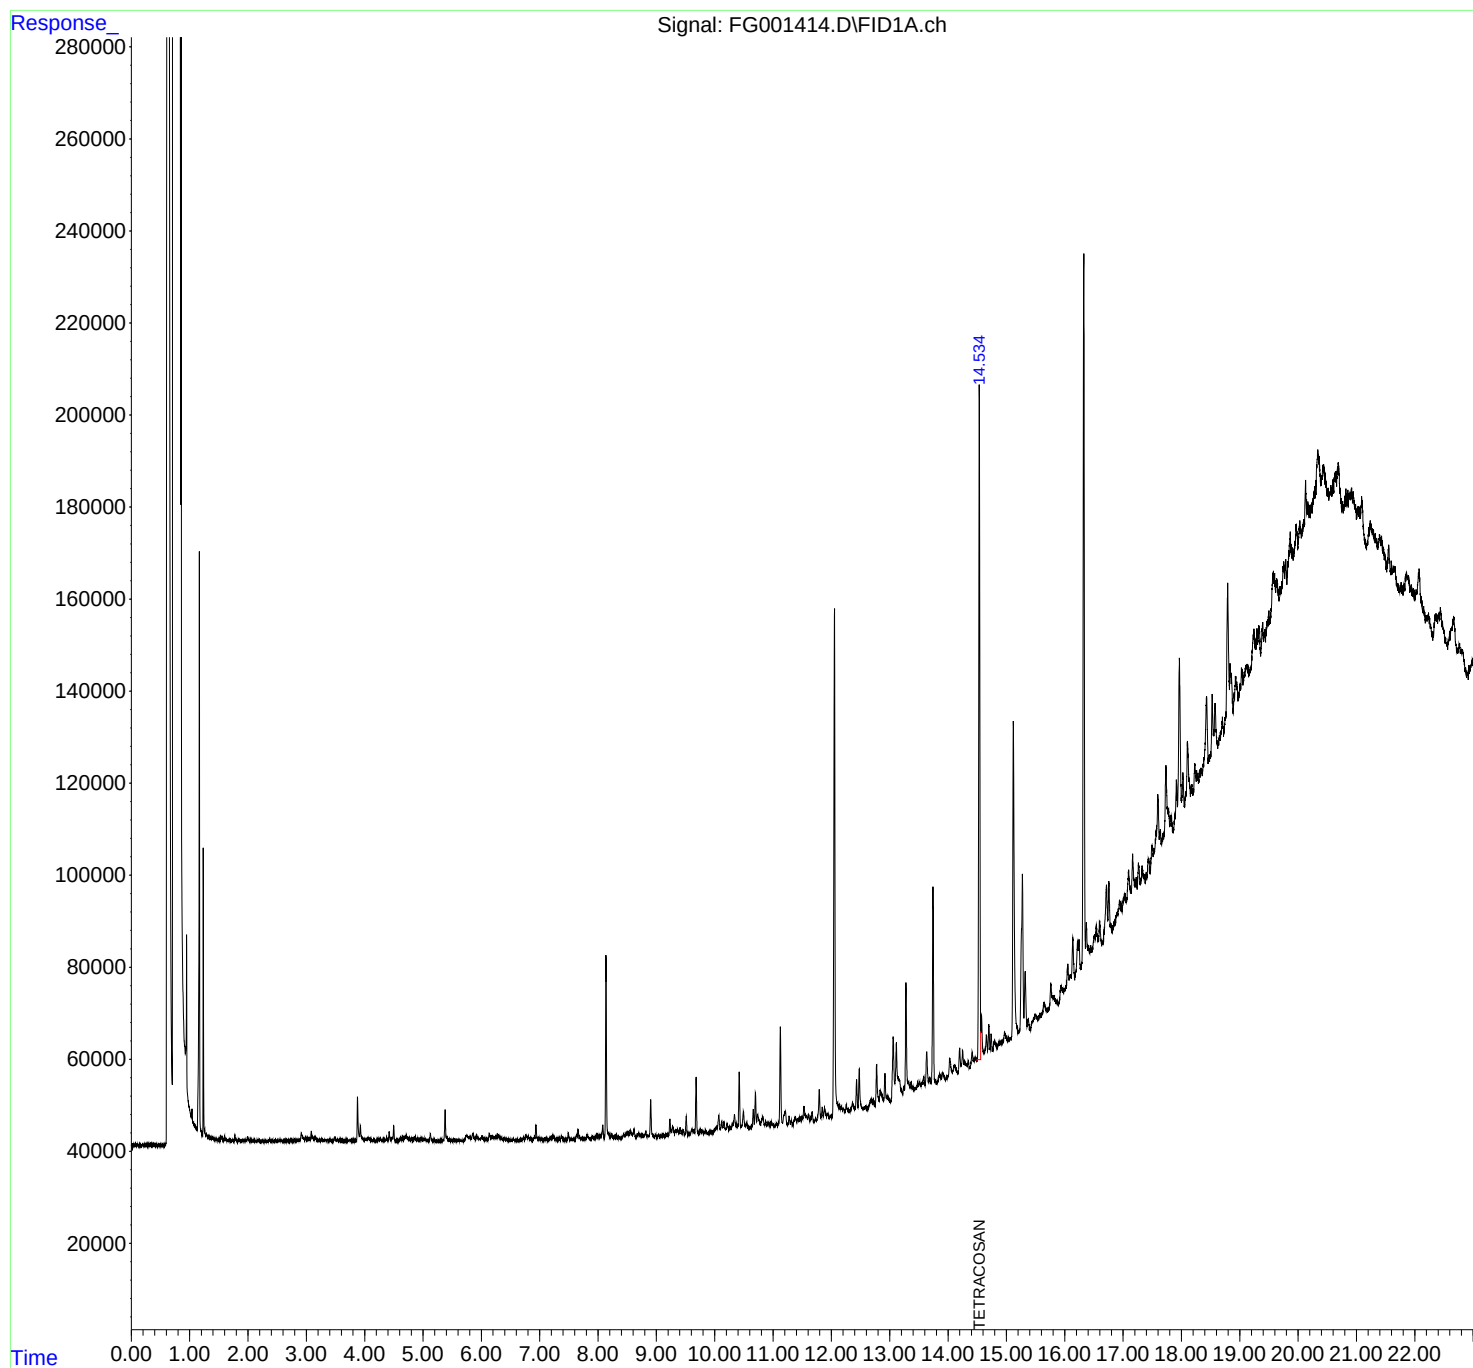

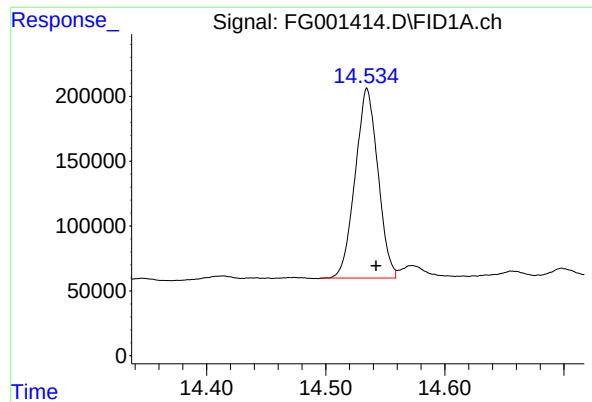

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.534 min
Delta R.T.: -0.008 min
Response: 1939340
Conc: 15.86 ug/ml m

Instrument :
FID_G
ClientSampleId :

Manual Integrations
APPROVED

UGO
6/21/2018 3:19:59 PM