

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062221\
Data File : FG008375.D
Signal(s) : FID1A.ch
Acq On : 22 Jun 2021 17:14
Operator : DD\AJ
Sample : M2791-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-02-20210618-A

Integration File: autoint1.e
Quant Time: Jun 23 00:53:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.771	1764788	14.871 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062221\
Data File : FG008375.D
Signal(s) : FID1A.ch
Acq On : 22 Jun 2021 17:14
Operator : DD\AJ
Sample : M2791-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-02-20210618-A

Integration File: autoint1.e
Quant Time: Jun 23 00:53:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

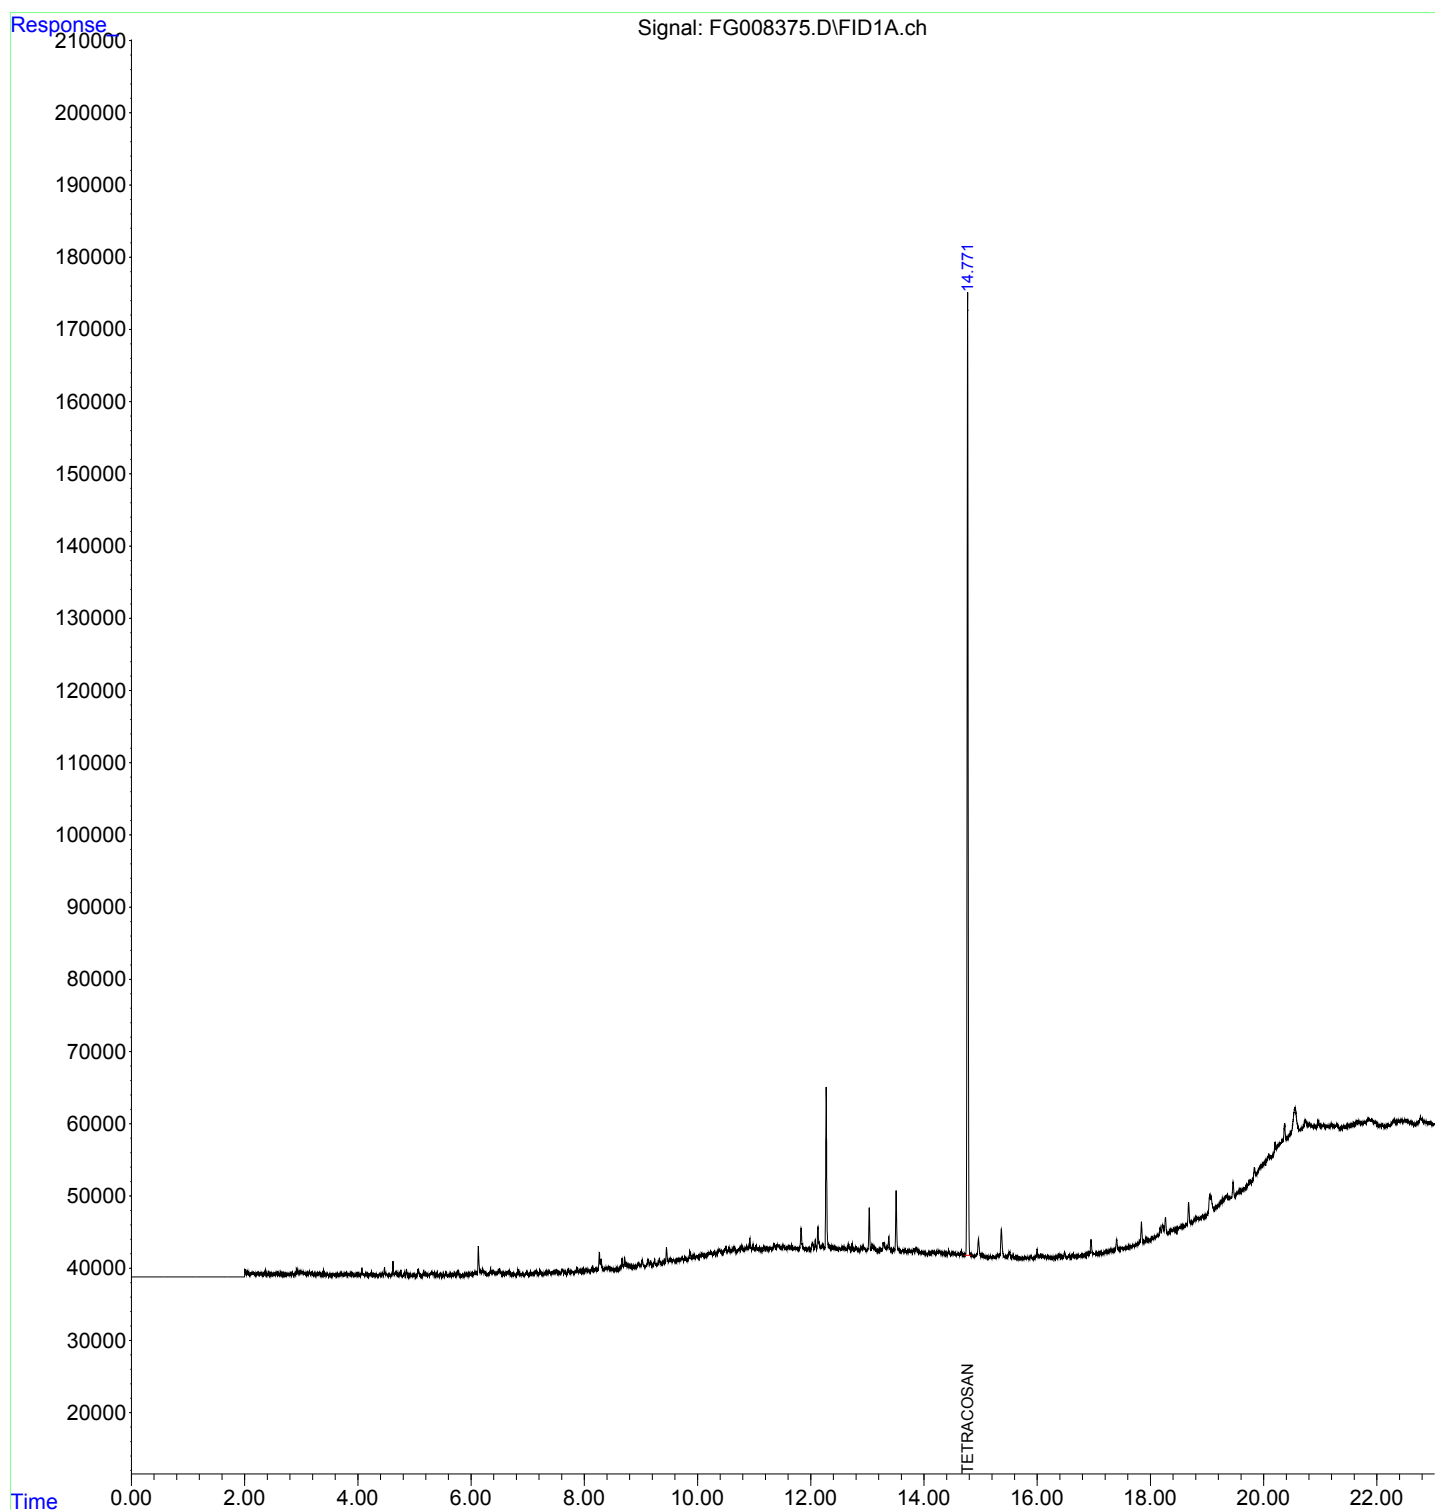

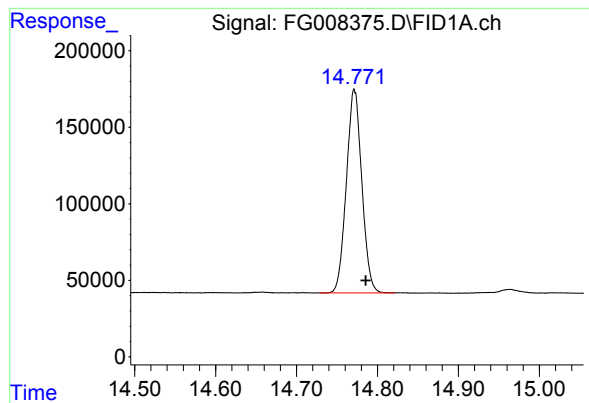

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.771 min
Delta R.T.: -0.014 min
Response: 1764788
Conc: 14.87 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-02-20210618-A