

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
 Data File : FG001457.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2018 14:50
 Operator : UA\AJ
 Sample : J3241-15 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 04:31:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.528	240235	1.965 ug/ml
Target Compounds			
3) N-DODECANE	6.286	246314	1.777 ug/ml
4) N-TETRADECANE	8.079	478284	3.423 ug/ml
5) N-HEXADECANE	9.678	410695	2.918 ug/ml
6) N-OCTADECANE	11.120	145124	1.024 ug/ml
7) N-EICOSANE	12.475	1733619	12.311 ug/ml
8) N-DOCOSANE	13.638	224309	1.601 ug/ml
10) N-TETRACOSANE	14.693f	709265	5.101 ug/ml
12) N-OCTACOSANE	16.696	184080	1.334 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
Data File : FG001457.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2018 14:50
Operator : UA\AJ
Sample : J3241-15 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 04:31:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

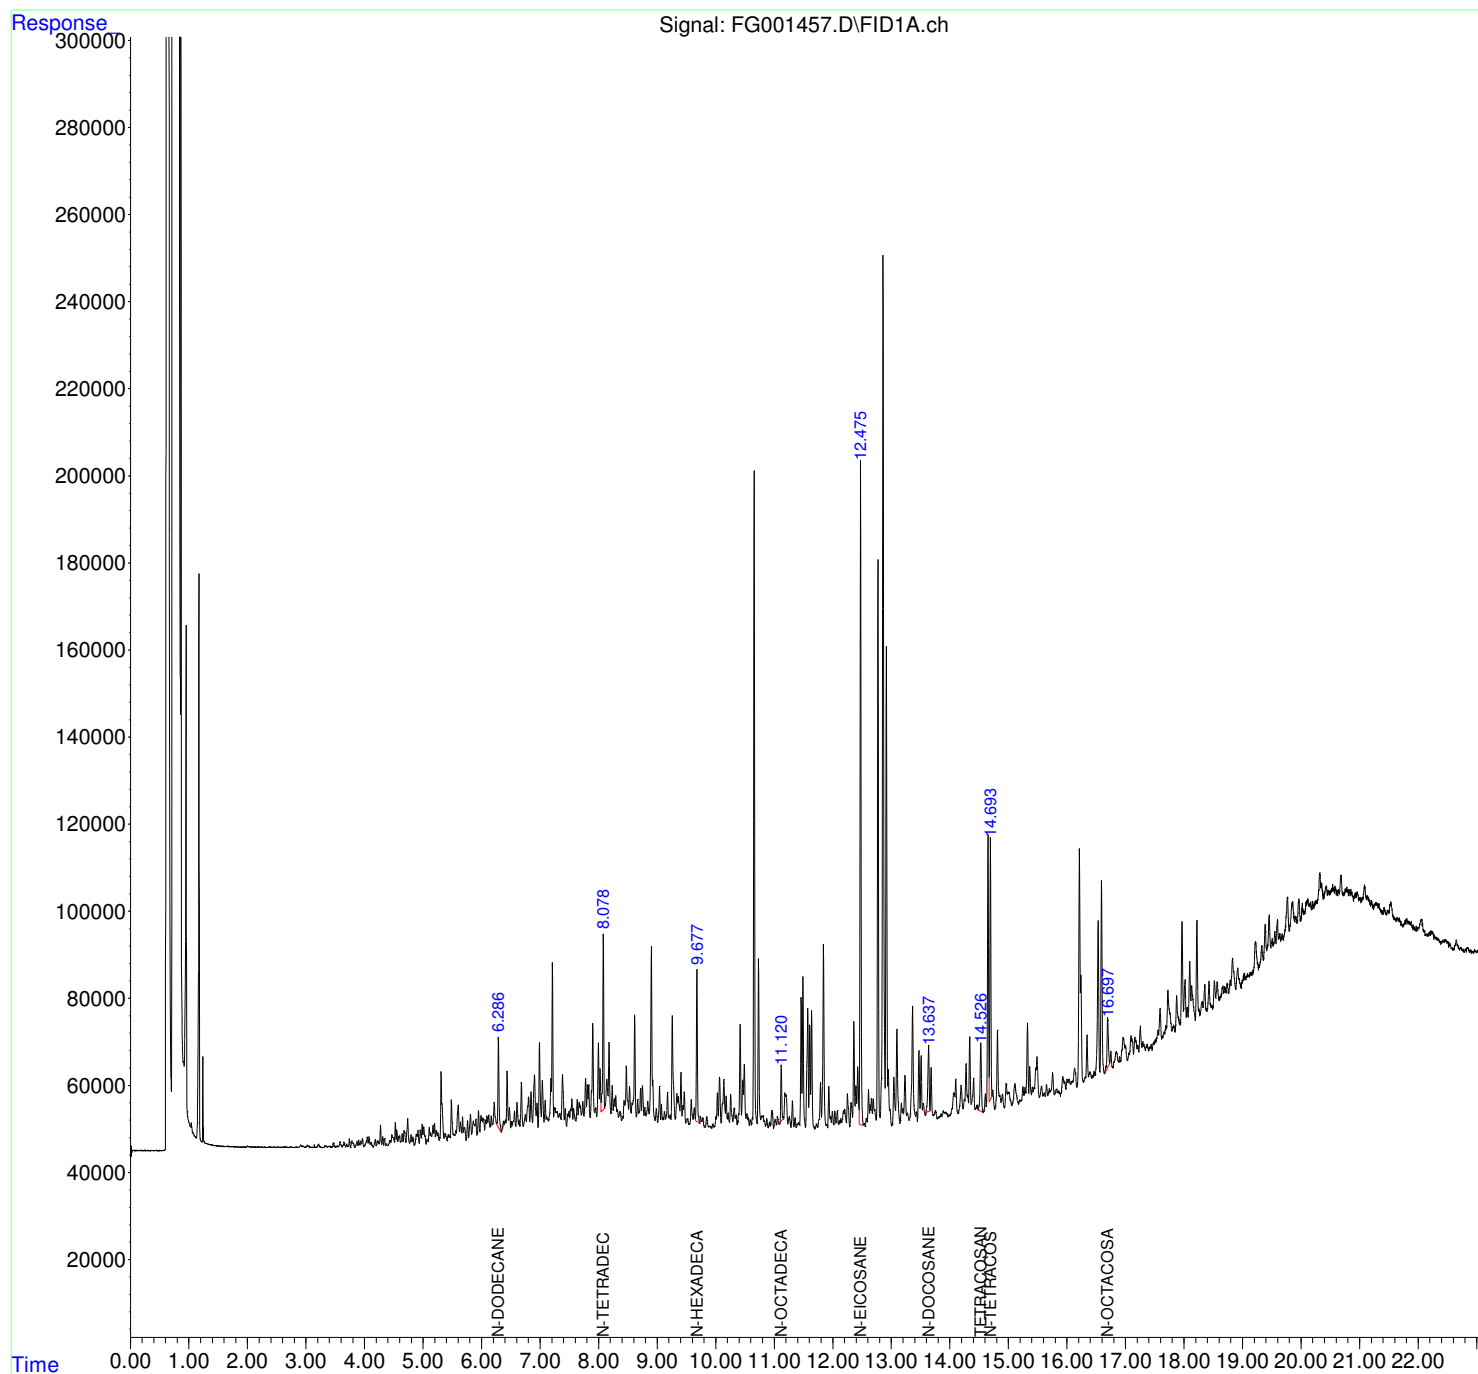


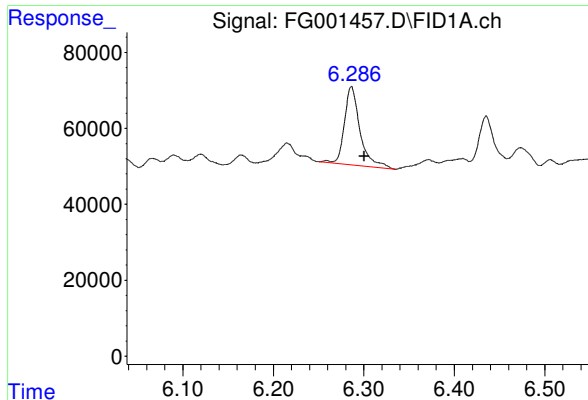

#3 N-DODECANE


R.T.: 6.286 min
Delta R.T.: -0.014 min
Response: 246314
Conc: 1.78 ug/ml

Instrument :
FID_G
ClientSampleId :

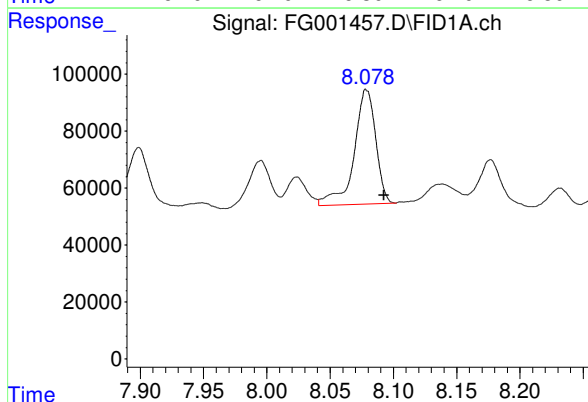


#4 N-TETRADECANE

R.T.: 8.079 min
Delta R.T.: -0.014 min
Response: 478284
Conc: 3.42 ug/ml

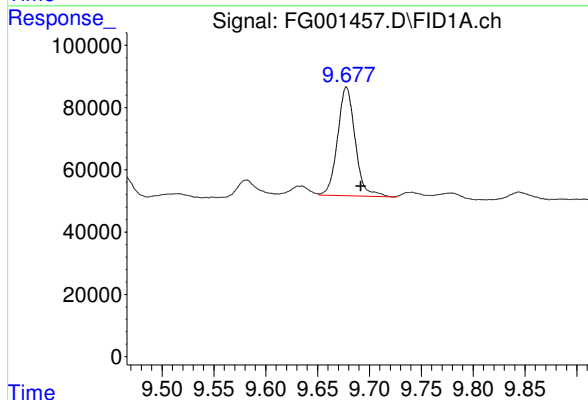


#5 N-HEXADECANE

R.T.: 9.678 min
Delta R.T.: -0.014 min
Response: 410695
Conc: 2.92 ug/ml

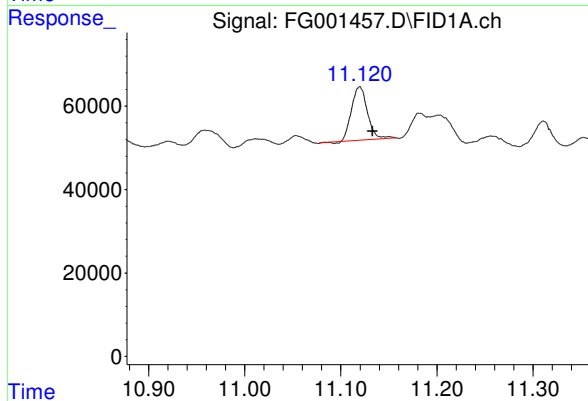

#6 N-OCTADECANE


R.T.: 11.120 min
Delta R.T.: -0.013 min
Response: 145124
Conc: 1.02 ug/ml

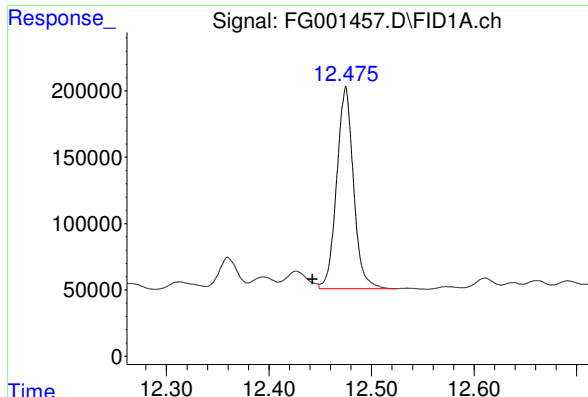

#7 N-EICOSANE


R.T.: 12.475 min
Delta R.T.: 0.032 min
Response: 1733619
Conc: 12.31 ug/ml

Instrument :
FID_G
ClientSampleId :

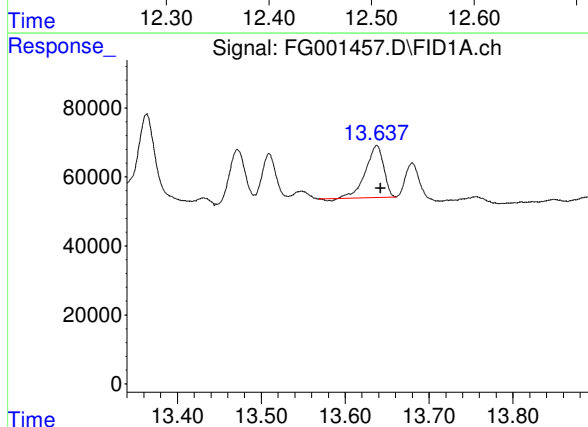


#8 N-DOCOSANE

R.T.: 13.638 min
Delta R.T.: -0.004 min
Response: 224309
Conc: 1.60 ug/ml

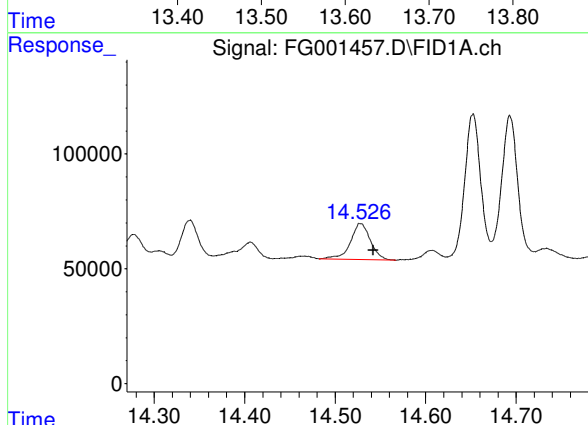


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.528 min
Delta R.T.: -0.014 min
Response: 240235
Conc: 1.97 ug/ml

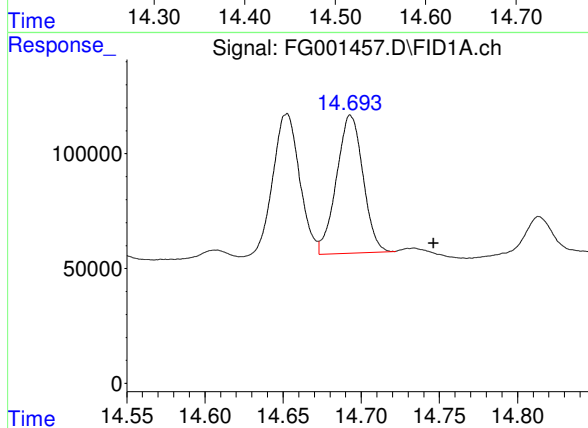

#10 N-TETRACOSANE

R.T.: 14.693 min
Delta R.T.: -0.053 min
Response: 709265
Conc: 5.10 ug/ml

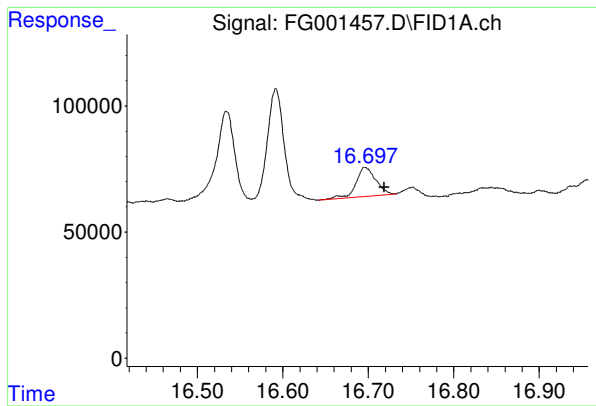

#12 N-OCTACOSANE

R.T.: 16.696 min
Delta R.T.: -0.023 min
Response: 184080
Conc: 1.33 ug/ml

Instrument :
FID_G
ClientSampleId :