

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
 Data File : FG001459.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2018 15:50
 Operator : UA\AJ
 Sample : J3252-03MS 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 04:31:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.530	659570	5.395 ug/ml
Target Compounds			
2) N-DECANE	4.272	183037	1.335 ug/ml
3) N-DODECANE	6.287	503027	3.629 ug/ml
4) N-TETRADECANE	8.079	569248	4.074 ug/ml
5) N-HEXADECANE	9.678	430487	3.059 ug/ml
6) N-OCTADECANE	11.119	261990	1.848 ug/ml
7) N-EICOSANE	12.431	274398	1.949 ug/ml
8) N-DOCOSANE	13.638	520434	3.713 ug/ml
10) N-TETRACOSANE	14.730	4395872	31.614 ug/ml
11) N-HEXACOSANE	15.757	252509	1.823 ug/ml
12) N-OCTACOSANE	16.708	317588	2.302 ug/ml
13) N-TRIACONTANE	17.597	341480	2.489 ug/ml
14) N-DOTRIACONTANE	18.433	823947	6.160 ug/ml
15) N-TETRATRIACONTANE	19.224	522520	3.966 ug/ml
16) N-HEXATRIACONTANE	19.966	317276	2.524 ug/ml
17) N-OCTATRIACONTANE	20.689	415048	3.662 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
Data File : FG001459.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2018 15:50
Operator : UA\AJ
Sample : J3252-03MS 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 04:31:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

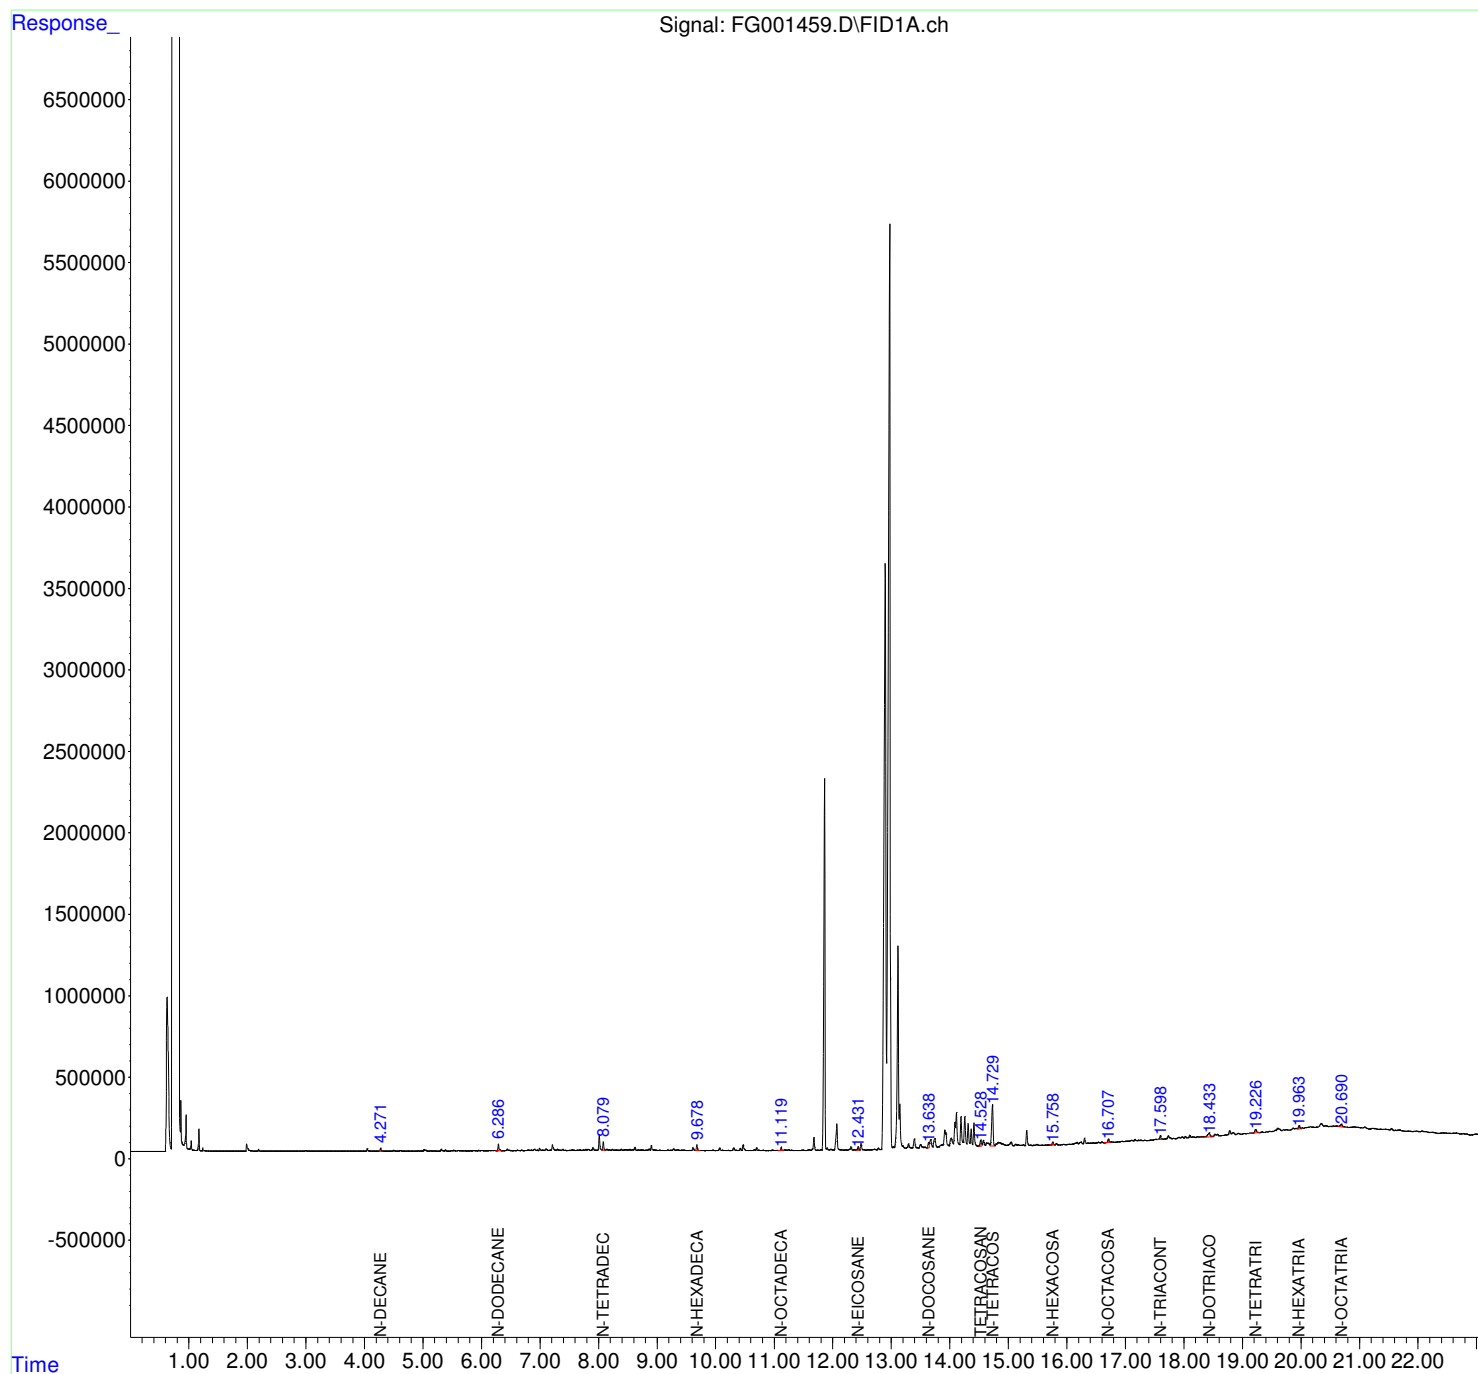


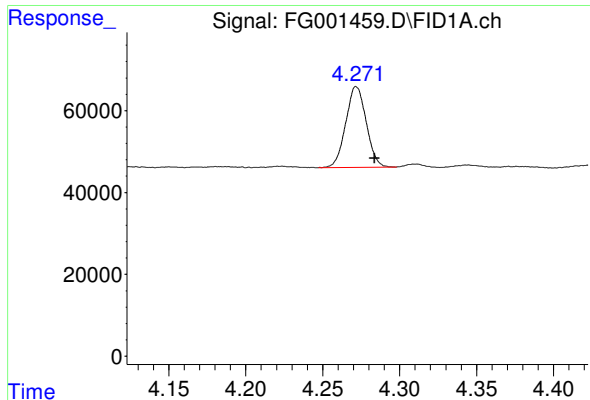

#2 N-DECANE


R.T.: 4.272 min
Delta R.T.: -0.012 min
Response: 183037
Conc: 1.34 ug/ml

Instrument :
FID_G
ClientSampleId :

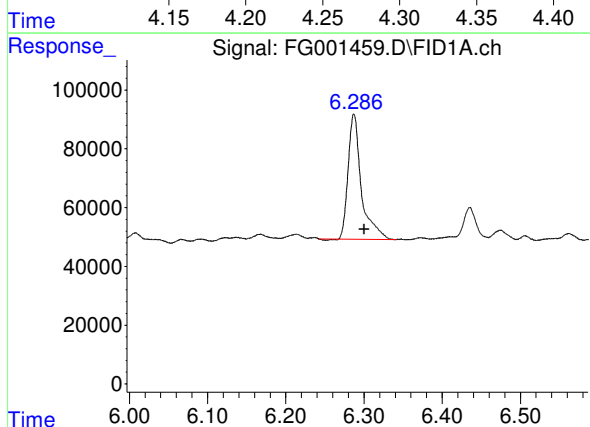


#3 N-DODECANE

R.T.: 6.287 min
Delta R.T.: -0.013 min
Response: 503027
Conc: 3.63 ug/ml

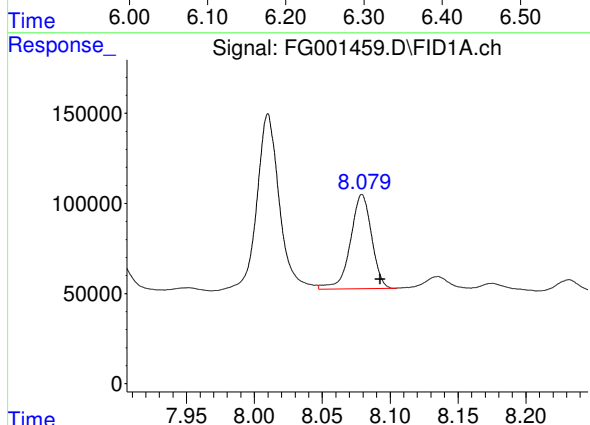


#4 N-TETRADECANE

R.T.: 8.079 min
Delta R.T.: -0.013 min
Response: 569248
Conc: 4.07 ug/ml

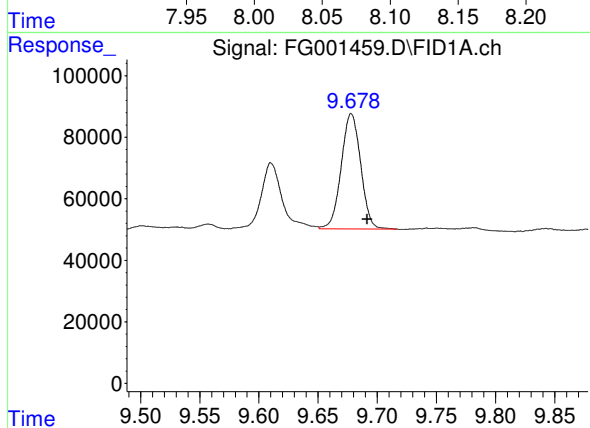

#5 N-HEXADECANE


R.T.: 9.678 min
Delta R.T.: -0.014 min
Response: 430487
Conc: 3.06 ug/ml

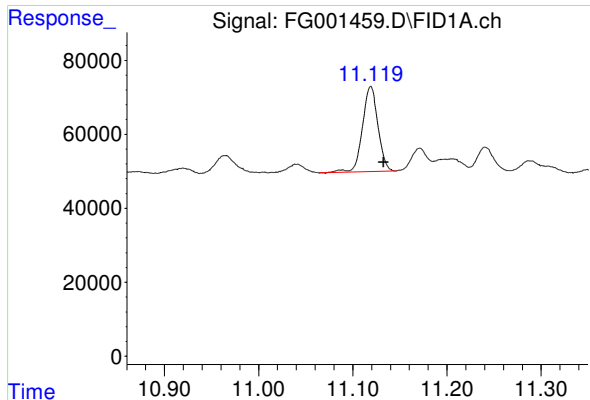

#6 N-OCTADECANE


R.T.: 11.119 min
Delta R.T.: -0.014 min
Response: 261990
Conc: 1.85 ug/ml

Instrument :
FID_G
ClientSampleId :

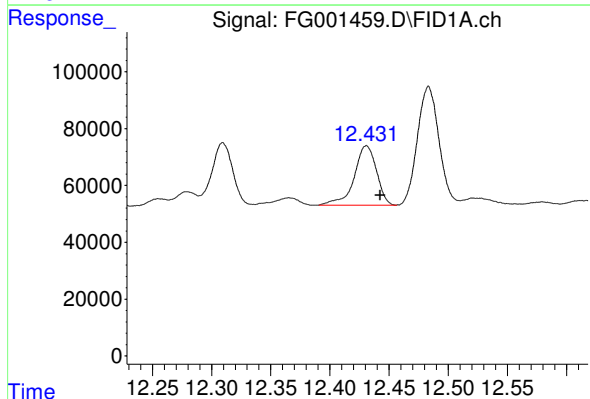


#7 N-EICOSANE

R.T.: 12.431 min
Delta R.T.: -0.012 min
Response: 274398
Conc: 1.95 ug/ml

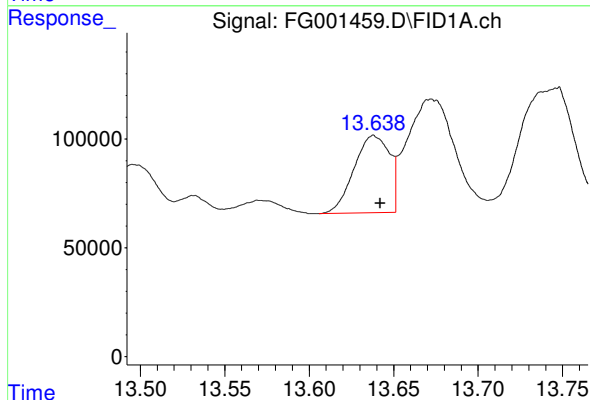


#8 N-DOCOSANE

R.T.: 13.638 min
Delta R.T.: -0.004 min
Response: 520434
Conc: 3.71 ug/ml

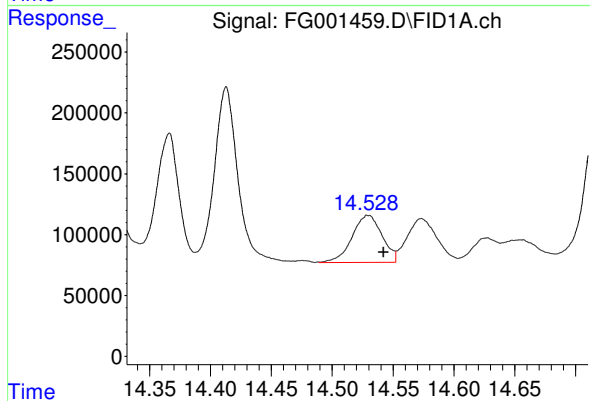

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.530 min
Delta R.T.: -0.013 min
Response: 659570
Conc: 5.40 ug/ml

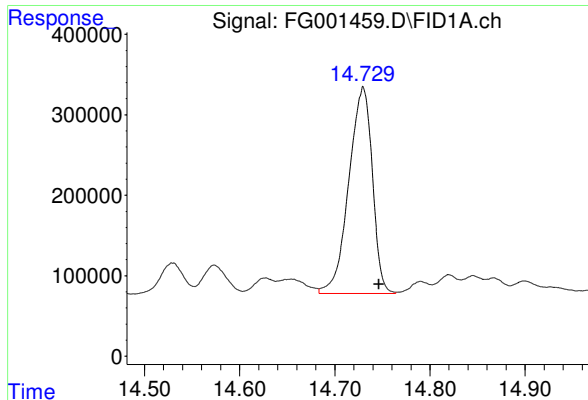

#10 N-TETRACOSANE


R.T.: 14.730 min
Delta R.T.: -0.016 min
Response: 4395872
Conc: 31.61 ug/ml

Instrument :
FID_G
ClientSampleId :

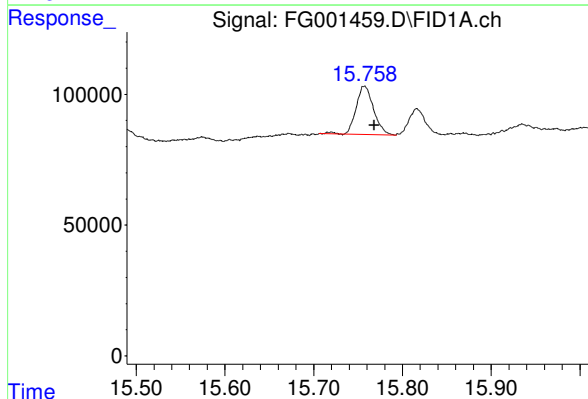


#11 N-HEXACOSANE

R.T.: 15.757 min
Delta R.T.: -0.011 min
Response: 252509
Conc: 1.82 ug/ml

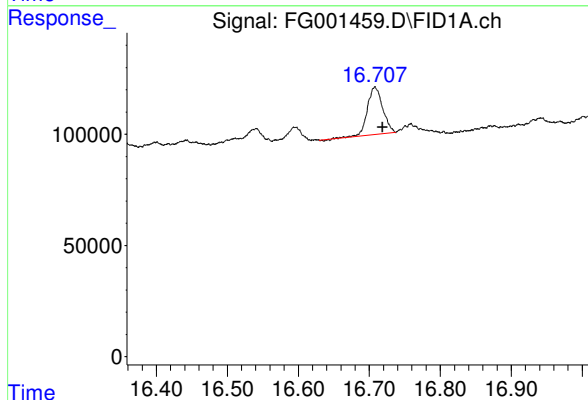


#12 N-OCTACOSANE

R.T.: 16.708 min
Delta R.T.: -0.011 min
Response: 317588
Conc: 2.30 ug/ml

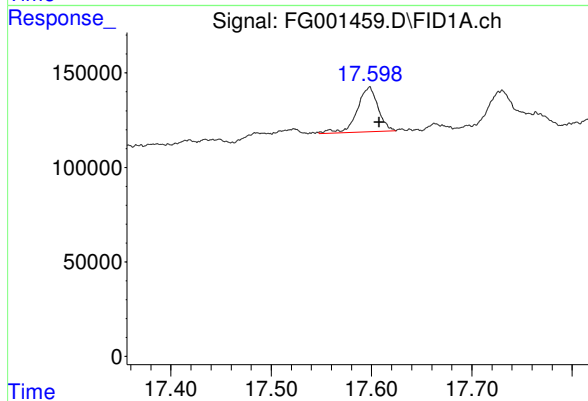

#13 N-TRIACONTANE


R.T.: 17.597 min
Delta R.T.: -0.010 min
Response: 341480
Conc: 2.49 ug/ml

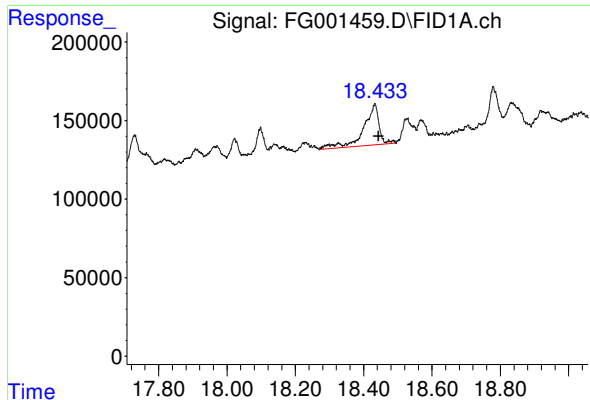

#14 N-DOTRIACONTANE


R.T.: 18.433 min
Delta R.T.: -0.011 min
Response: 823947
Conc: 6.16 ug/ml

Instrument :
FID_G
ClientSampleId :

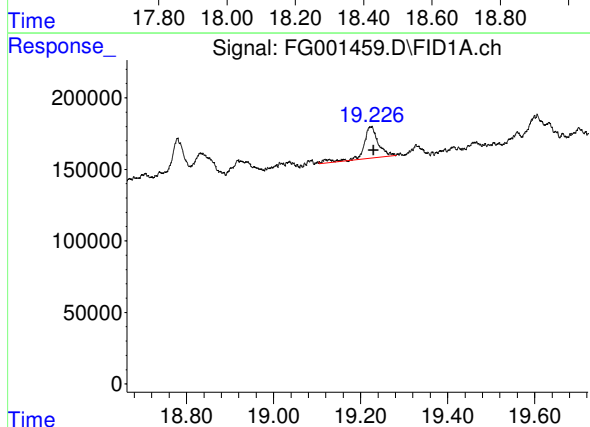


#15 N-TETRATRIACONTANE

R.T.: 19.224 min
Delta R.T.: -0.006 min
Response: 522520
Conc: 3.97 ug/ml

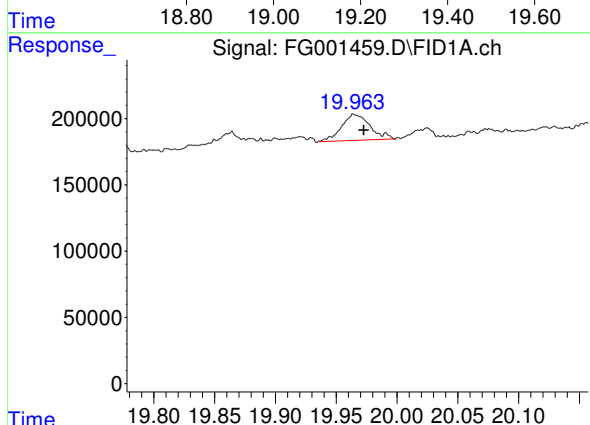

#16 N-HEXATRIACONTANE

R.T.: 19.966 min
Delta R.T.: -0.007 min
Response: 317276
Conc: 2.52 ug/ml

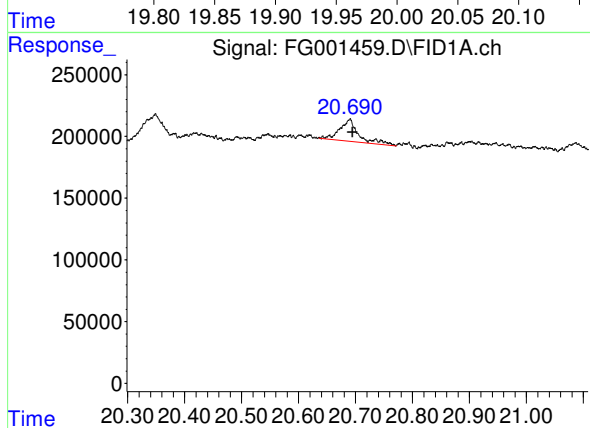

#17 N-OCTATRIACONTANE

R.T.: 20.689 min
Delta R.T.: -0.005 min
Response: 415048
Conc: 3.66 ug/ml